

(12) **United States Patent**
Dagum et al.

(10) **Patent No.:** **US 12,133,738 B2**

(45) **Date of Patent:** **Nov. 5, 2024**

(54) **NON-INVASIVE TOPOGRAPHIC
LOCALIZATION OF GLYMPHATIC FLOW**

(71) Applicant: **Applied Cognition, Inc.**, Los Altos
 Hills, CA (US)

(72) Inventors: **Paul Dagum**, Los Altos Hills, CA (US);
 Laurent B. Giovangrandi, Palo Alto,
 CA (US)

(73) Assignee: **Applied Cognition, Inc.**, Redwood
 City, CA (US)

(*) Notice: Subject to any disclaimer, the term of this
 patent is extended or adjusted under 35
 U.S.C. 154(b) by 26 days.

(21) Appl. No.: **18/492,775**

(22) Filed: **Oct. 23, 2023**

(65) **Prior Publication Data**

US 2024/0130664 A1 Apr. 25, 2024
US 2024/0225523 A9 Jul. 11, 2024

Related U.S. Application Data

(60) Provisional application No. 63/380,726, filed on Oct.
24, 2022.

(51) **Int. Cl.**
 A61B 5/00 (2006.01)
 A61B 5/0536 (2021.01)
 (Continued)

(52) **U.S. Cl.**
 CPC **A61B 5/4064** (2013.01); **A61B 5/0536**
 (2013.01); **A61B 5/256** (2021.01);
 (Continued)

(58) **Field of Classification Search**
 CPC A61B 5/4064; A61B 5/0536; A61B 5/256;
 A61B 5/4088; A61B 5/6814
 See application file for complete search history.

(56) **References Cited**

 U.S. PATENT DOCUMENTS

6,511,437 B1 1/2003 Nakamura
6,640,121 B1 10/2003 Telischi et al.
 (Continued)

 FOREIGN PATENT DOCUMENTS

WO 2019169142 9/2019
WO 2020035852 2/2020
 (Continued)

 OTHER PUBLICATIONS


Goverdovsky et al, “In-Ear EEG From Viscoelastic Generic Earpieces:
Robust and Unobtrusive 24/7 Monitoring”, IEEE Sensors Journal,
Jan. 1, 2016, pp. 271-277, vol. 16, No. 1.
 (Continued)

Primary Examiner — Eugene T Wu
(74) Attorney, Agent, or Firm — King & Spalding LLP

(57) **ABSTRACT**

A computer-implemented method and system includes
accessing neurophysiological and neurovascular data
recorded during sleep. A device mounted on a subject’s head
during sleep can gather neurovascular data by measuring
transcranial impedance. The device can be in the form of a
single band, multiple bands, or a headcap that are worn on
the subject’s head. Electrodes located along an inner surface
of the wearable device contact the subject’s head and
measure transcranial impedance. Transcranial impedance
measurements are gathered from multiple locations on the
subject’s head and over multiple frequencies to obtain a
more complete assessment of glymphatic flow.

7 Claims, 39 Drawing Sheets

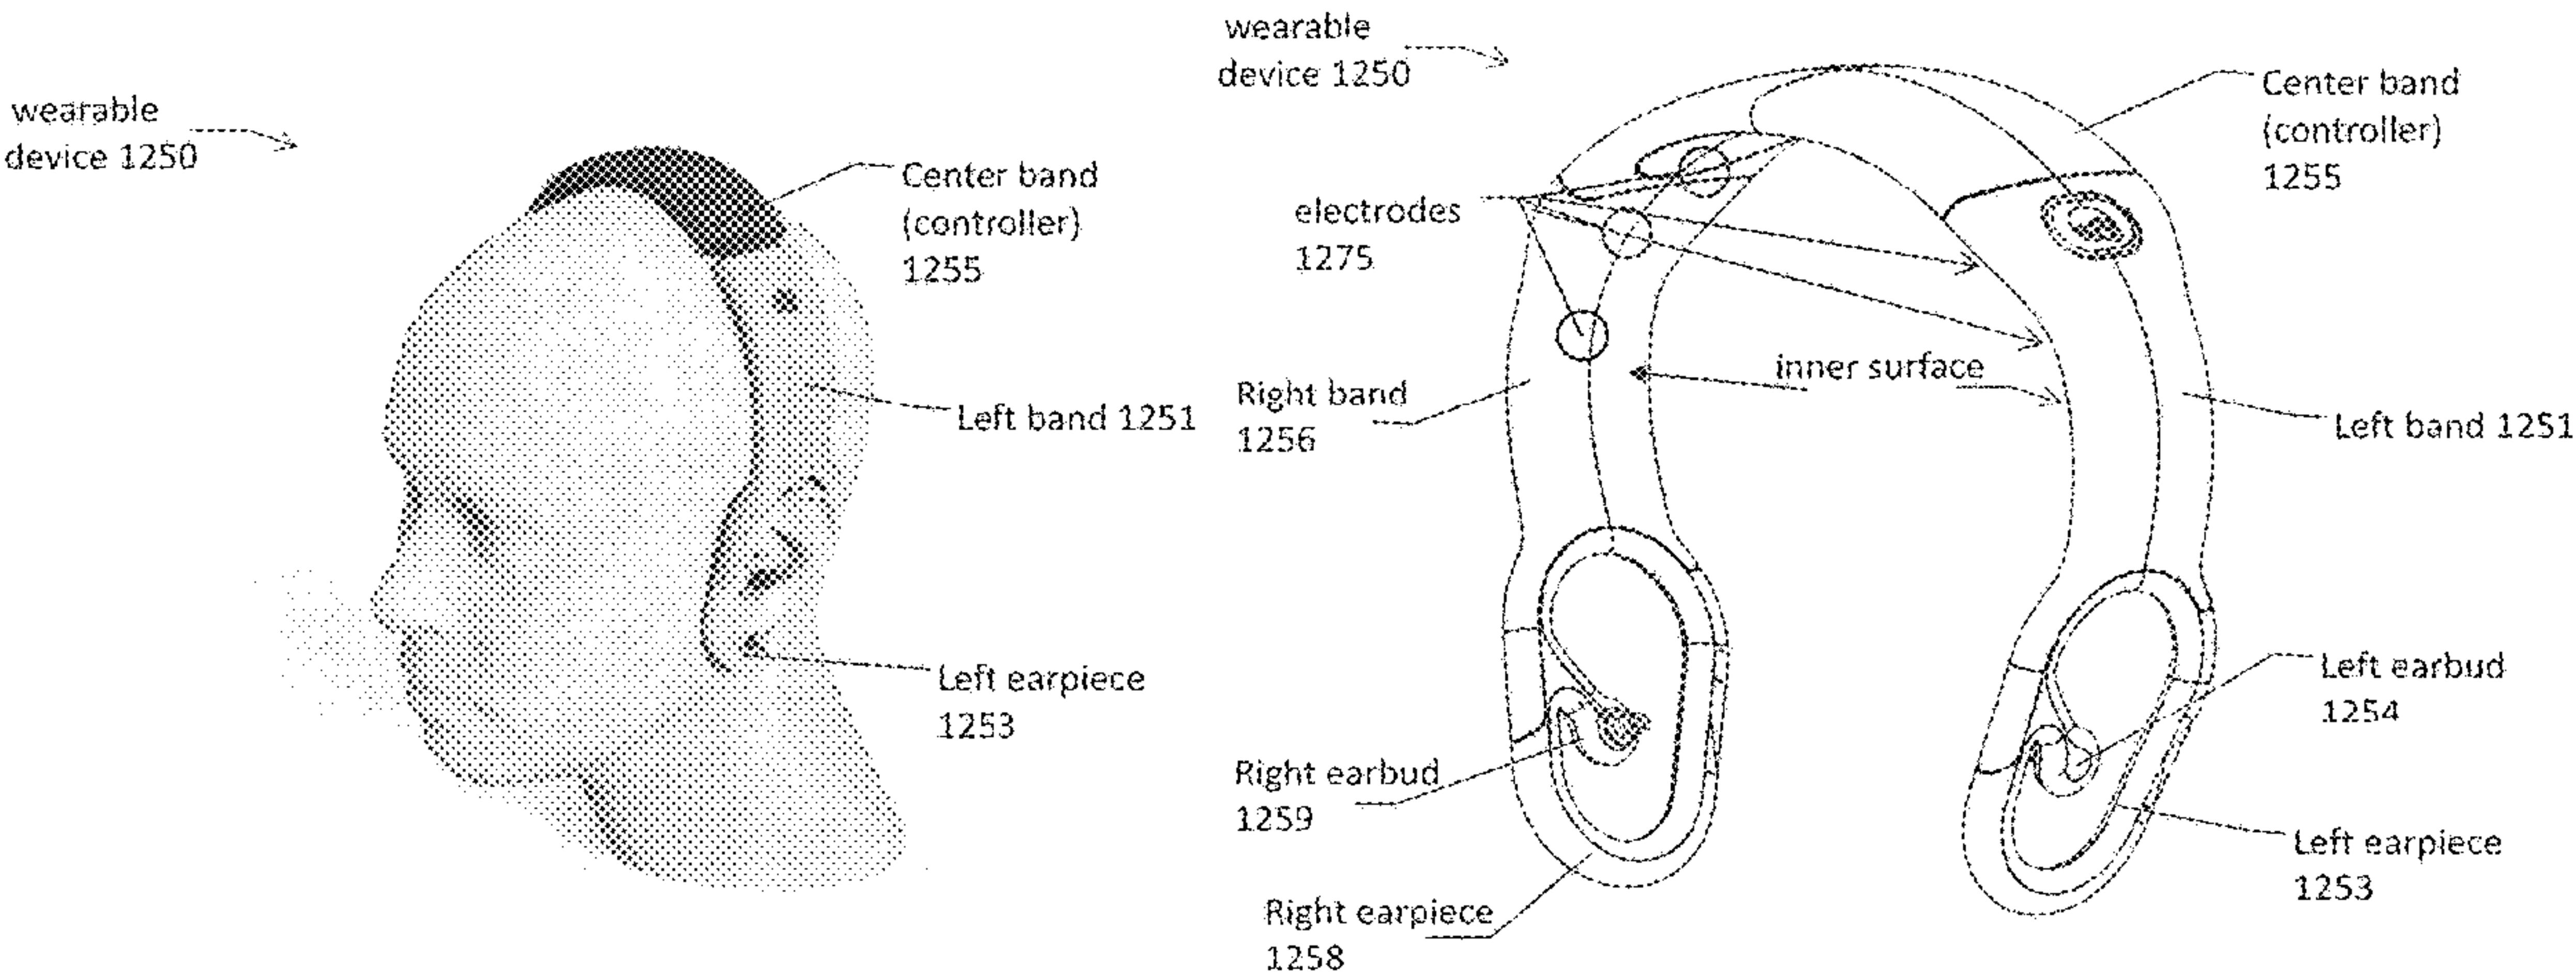

- (51) **Int. Cl.**
A61B 5/256 (2021.01)
A61M 21/02 (2006.01)
A61N 1/05 (2006.01)
- (52) **U.S. Cl.**
CPC *A61B 5/4088* (2013.01); *A61B 5/6814*
(2013.01); *A61B 5/6817* (2013.01); *A61M*
21/02 (2013.01); *A61N 1/0541* (2013.01)

(56) **References Cited**

U.S. PATENT DOCUMENTS

7,209,775	B2	4/2007	Bae et al.	
8,277,385	B2	10/2012	Berka	
8,884,767	B2	11/2014	Kidmose	
8,926,542	B2	1/2015	Gerber	
9,025,800	B2	5/2015	Kidmose et al.	
9,210,517	B2	12/2015	Pontoppidan et al.	
9,307,918	B2	4/2016	Kinrot	
9,408,552	B2	8/2016	Kidmose et al.	
9,918,650	B2	3/2018	Kilsgaard et al.	
9,949,045	B2	4/2018	Kure et al.	
10,052,065	B2	8/2018	Boesen	
10,194,228	B2	1/2019	Hirsch	
10,275,027	B2	4/2019	Segal	
10,433,788	B2	10/2019	Boesen	
10,542,904	B2	1/2020	Durand	
10,575,777	B2	3/2020	Ayers et al.	
10,606,354	B2	3/2020	Segal	
10,617,297	B2	4/2020	Turner	
10,728,642	B2	7/2020	Solum et al.	
10,743,121	B2	8/2020	Pontoppidan et al.	
10,765,337	B2	9/2020	Andersen	
10,798,487	B2	10/2020	Hviid	
10,835,145	B1	11/2020	Prevoir et al.	
10,841,682	B2	11/2020	Masaki et al.	
10,856,063	B1	12/2020	Hviid	
10,856,071	B2	12/2020	Verdooner et al.	
11,298,542	B2	4/2022	Aur	
11,478,184	B1	10/2022	Dagum	
11,759,142	B2 *	9/2023	Dagum A61B 5/0006 600/544	
2007/0112277	A1	5/2007	Fischer et al.	
2007/0287899	A1	12/2007	Poupko	
2009/0264776	A1	10/2009	Vardy	
2011/0196245	A1	8/2011	Poupko	
2011/0251503	A1	10/2011	Ben-Ari	
2012/0165695	A1	6/2012	Kidmose et al.	
2012/0302858	A1	11/2012	Kidmose et al.	
2013/0085356	A1	4/2013	Schlottau	
2014/0018649	A1	1/2014	Jespersen	
2016/0000945	A1 *	1/2016	Nedergaard A61P 25/16 604/9	
2016/0022195	A1	1/2016	Vardy	
2016/0199203	A1 *	7/2016	Adachi A61F 2/72 600/383	
2016/0310028	A1	10/2016	Kidmose et al.	
2016/0317085	A1	11/2016	Razavi	
2016/0367166	A1 *	12/2016	Piron A61B 5/031	
2017/0224949	A1	8/2017	Action	
2017/0251950	A1	9/2017	Piron et al.	
2017/0311870	A1	11/2017	Bardakjian et al.	
2017/0311881	A1	11/2017	Jensen et al.	
2017/0312518	A1 *	11/2017	Ziegler A61B 5/0075	
2018/0014741	A1	1/2018	Chou	
2018/0055398	A1	3/2018	Westermann et al.	
2018/0177421	A1	6/2018	Kilsgaard et al.	
2018/0220903	A1	8/2018	LeBoeuf et al.	
2018/0228381	A1	8/2018	LeBoeuf et al.	
2018/0235540	A1	8/2018	Kirszenblat et al.	
2018/0271428	A1	9/2018	Takagi et al.	

2018/0277238	A1	9/2018	Boesen	
2018/0277245	A1	9/2018	Boesen	
2018/0353095	A1	12/2018	Boesen	
2018/0368718	A1	12/2018	Koziol	
2019/0174238	A1	6/2019	Lunner et al.	
2019/0209038	A1	7/2019	Saab et al.	
2019/0223747	A1	7/2019	Chou	
2019/0253793	A1	8/2019	Pedersen et al.	
2019/0269336	A1	9/2019	Perkins et al.	
2019/0282119	A1	9/2019	Andersen et al.	
2019/0380597	A1	12/2019	Howard	
2020/0085331	A1	3/2020	Chou	
2020/0225750	A1	7/2020	Segal	
2020/0268265	A1	8/2020	Walsh et al.	
2020/0288253	A1	9/2020	De Haan et al.	
2020/0297211	A1 *	9/2020	Jordan G16H 10/60	
2020/0306493	A1	10/2020	Lee	
2021/0241909	A1	8/2021	Bulut	
2021/0275097	A1	9/2021	Pushpala	
2021/0282698	A1	9/2021	Garcia Molina	
2022/0000421	A1	1/2022	Ippolito	

FOREIGN PATENT DOCUMENTS

WO	2020061209	3/2020
WO	2020127940	6/2020
WO	2020210813	10/2020
WO	WO 2022-180306	A2 9/2022

OTHER PUBLICATIONS

Goverdovsky et al. "Hearables: Multimodal physiological in-ear sensing", Scientific Reports, Jul. 31, 2017, pp. 1-10, 7: 6948 | DOI: 10.1038/s41598-017-06925-2.

R. Kusche et al., "An in-ear pulse wave velocity measurement system using heart sounds as time reference", Current Directions in Biomedical Engineering 2015; 1:366-370, De Gruyter.

Kwon, Shinjae, Hojoong Kim, and Woon-Hong Yeo; "Recent Advances In Wearable Sensors and Portable Electronics for Sleep Monitoring"; iScience 24.5 (2021): 102461 (Year: 2021).

Hablitz, Lauren M., et al.; "Increased Glymphatic Influx Is Correlated With Hight EEG Delta Power and Low Heart Rate in Mice Under Anesthesia"; Science Advances 5.2 (2019); eaav5447; (Year: 2019).

Tanabe, Sean, et al. "Cohort Study of Electroencephalography Markers of Amyloid-Tau-Neurodegeneration Pathology."; Brain Communications 2.2 (2020): fcaa099. (Year:2020).

International Search Report and Written Opinion issued in PCT Application No. PCT/US2022/023409, mailed Jul. 25, 2022, 9 pages, Korean Intellectual Property Office.

Meghdadi, et al., "Transcranial Impedance Changes During Sleep: A Rheoencephalography Study," IEEE Journal of Translational Engineering in Health and Medicine, vol. 7, 2019.

Guermandi, Marco, et al., "Active Electrode IC for EEG and Electrical Impedance Tomography With Continuous Monitoring of Contact Impedance," IEEE Transactions on Biomedical Circuits and Systems, vol. 9, No. 1, Feb. 2015.

International Search Report and Written Opinion for PCT Patent Application No. PCT/US2023/077566 dated Feb. 19, 2024.

International Search Report and Written Opinion for PCT Patent Application No. PCT/US2023/077562 dated Feb. 19, 2024.

Moskalenko, Yu; Multifrequency REG: Fundamental Background, Information Meaning and Ways of Data Analysis and Automation; Am. J. Biomedical Eng'g; 2012; 2(4): 163-174.

Taoka, Taoshiaki; Neurofluid Dynamics and the Glymphatic System: A Neuroimaging Perspective; Korean J. of Radiology; 2020; 21(11):1199-1209.

* cited by examiner

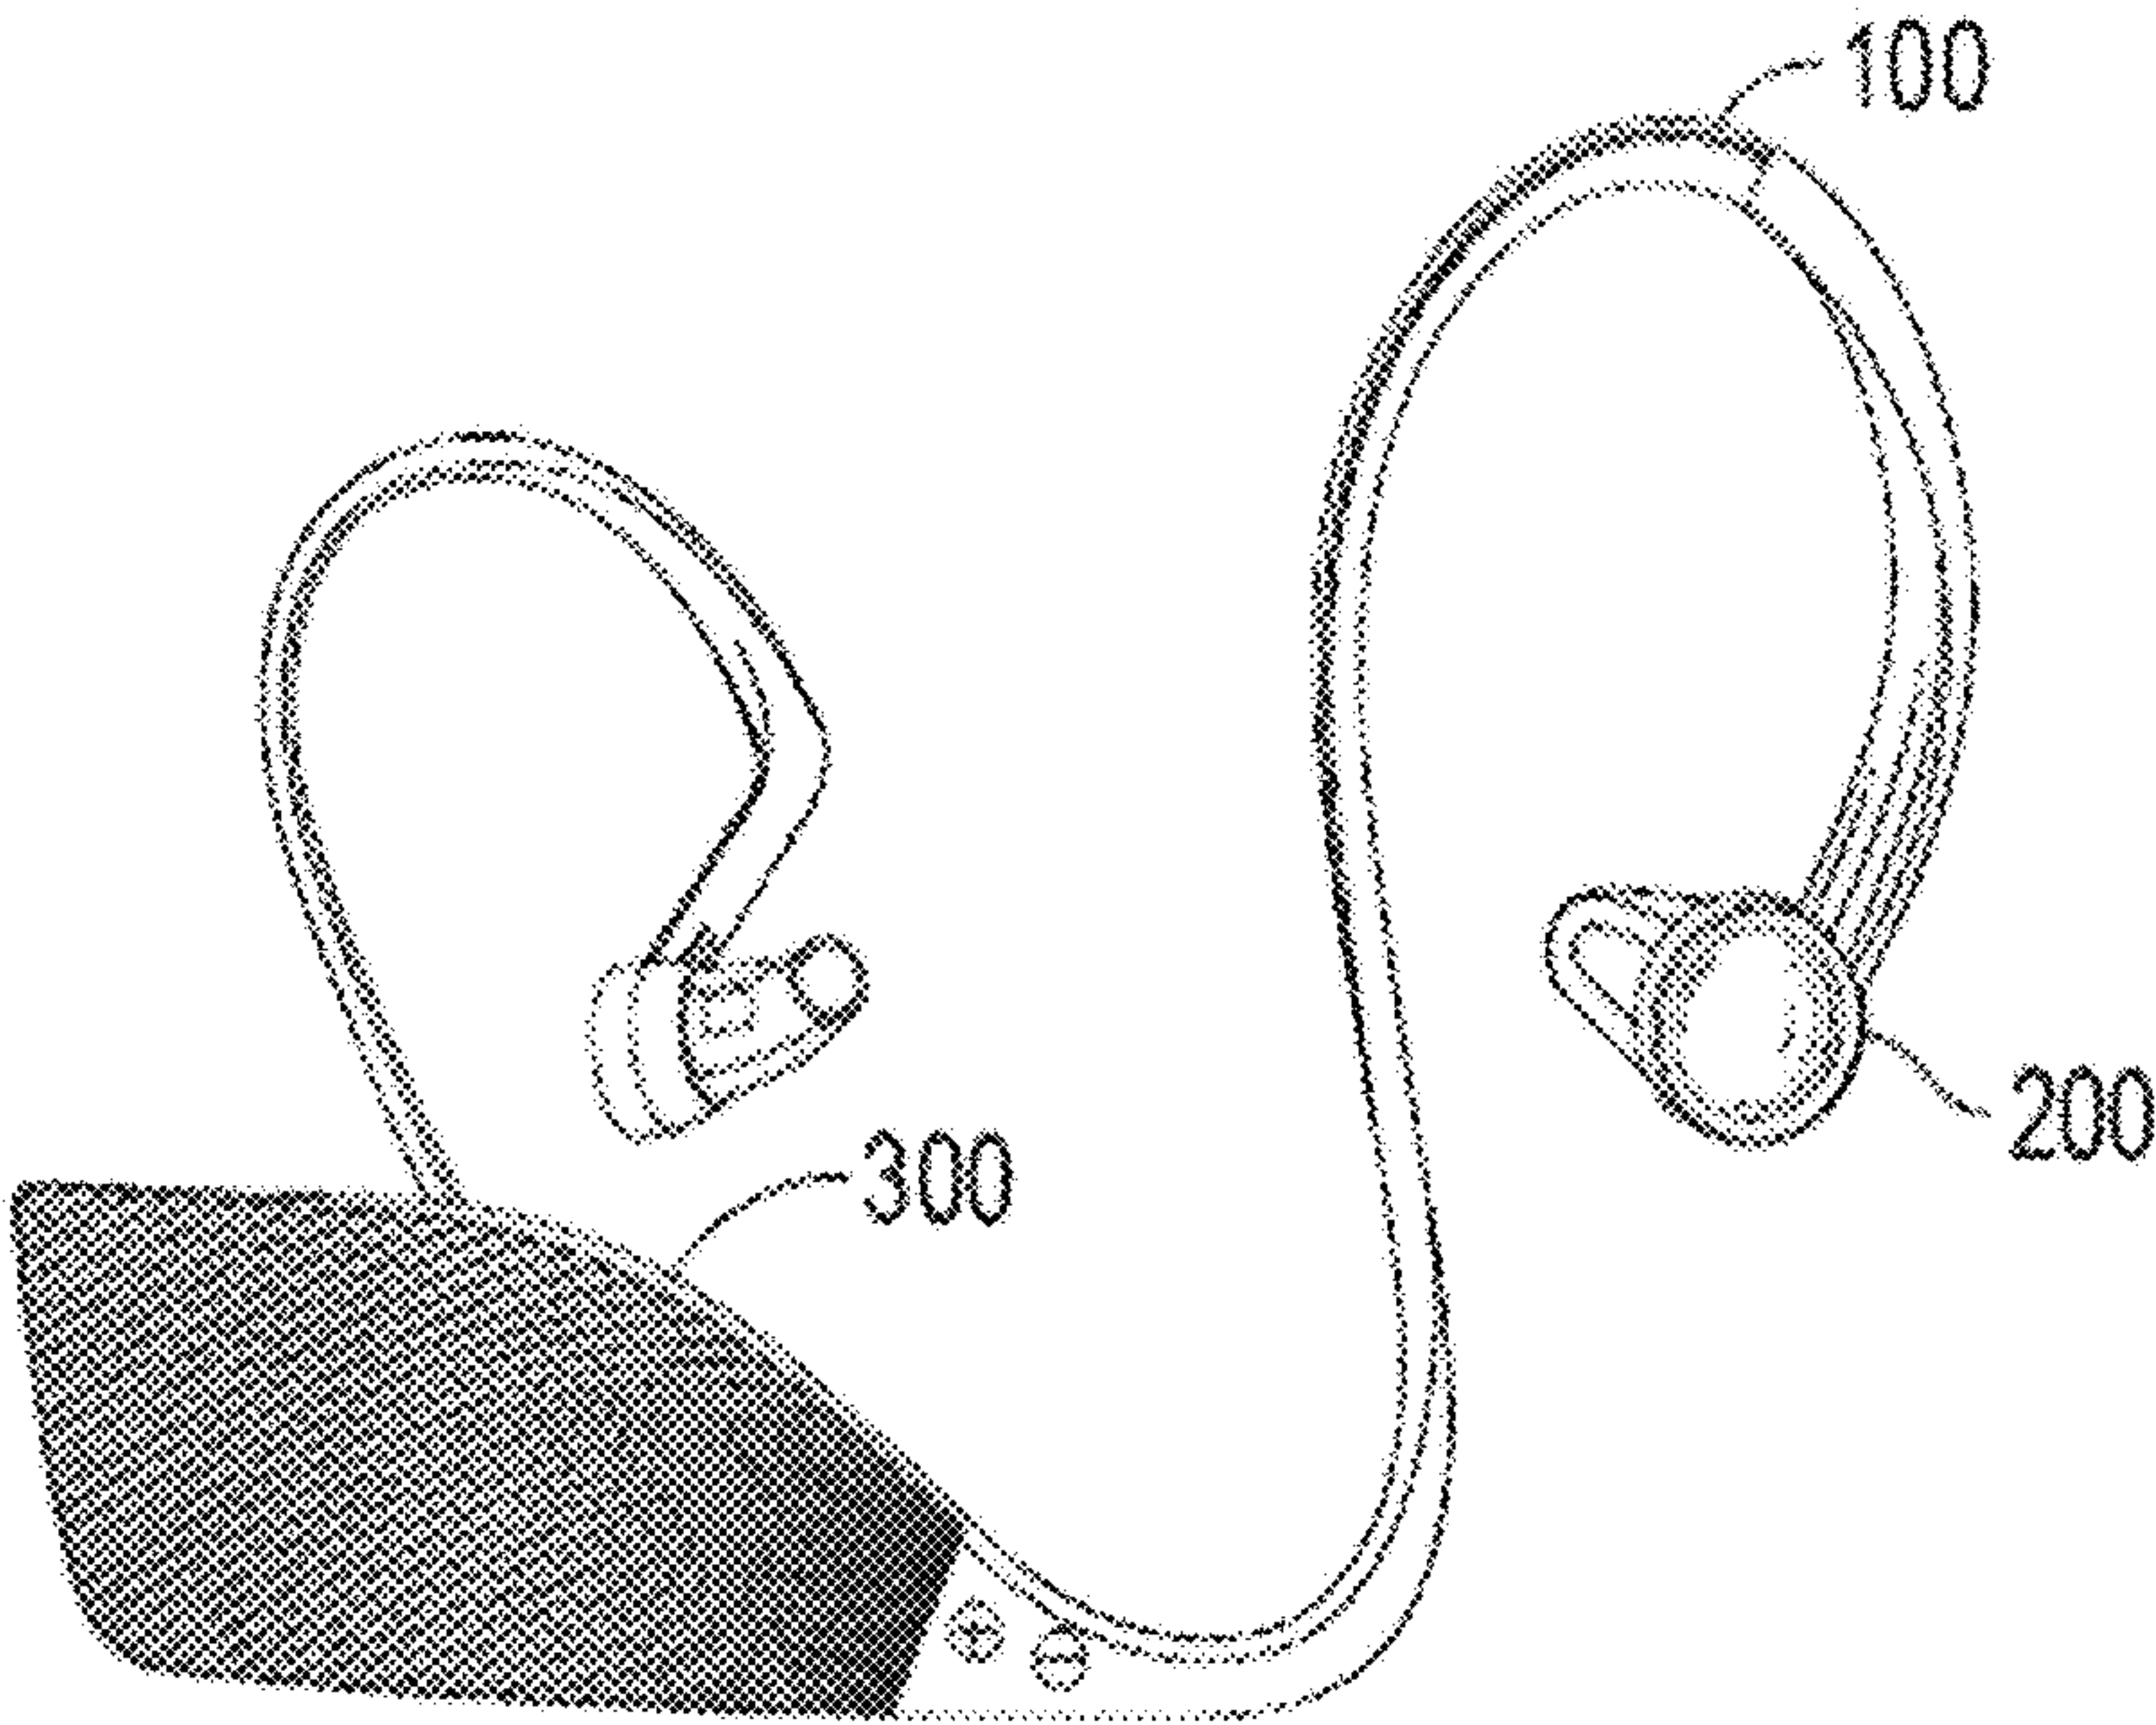


FIG. 1A

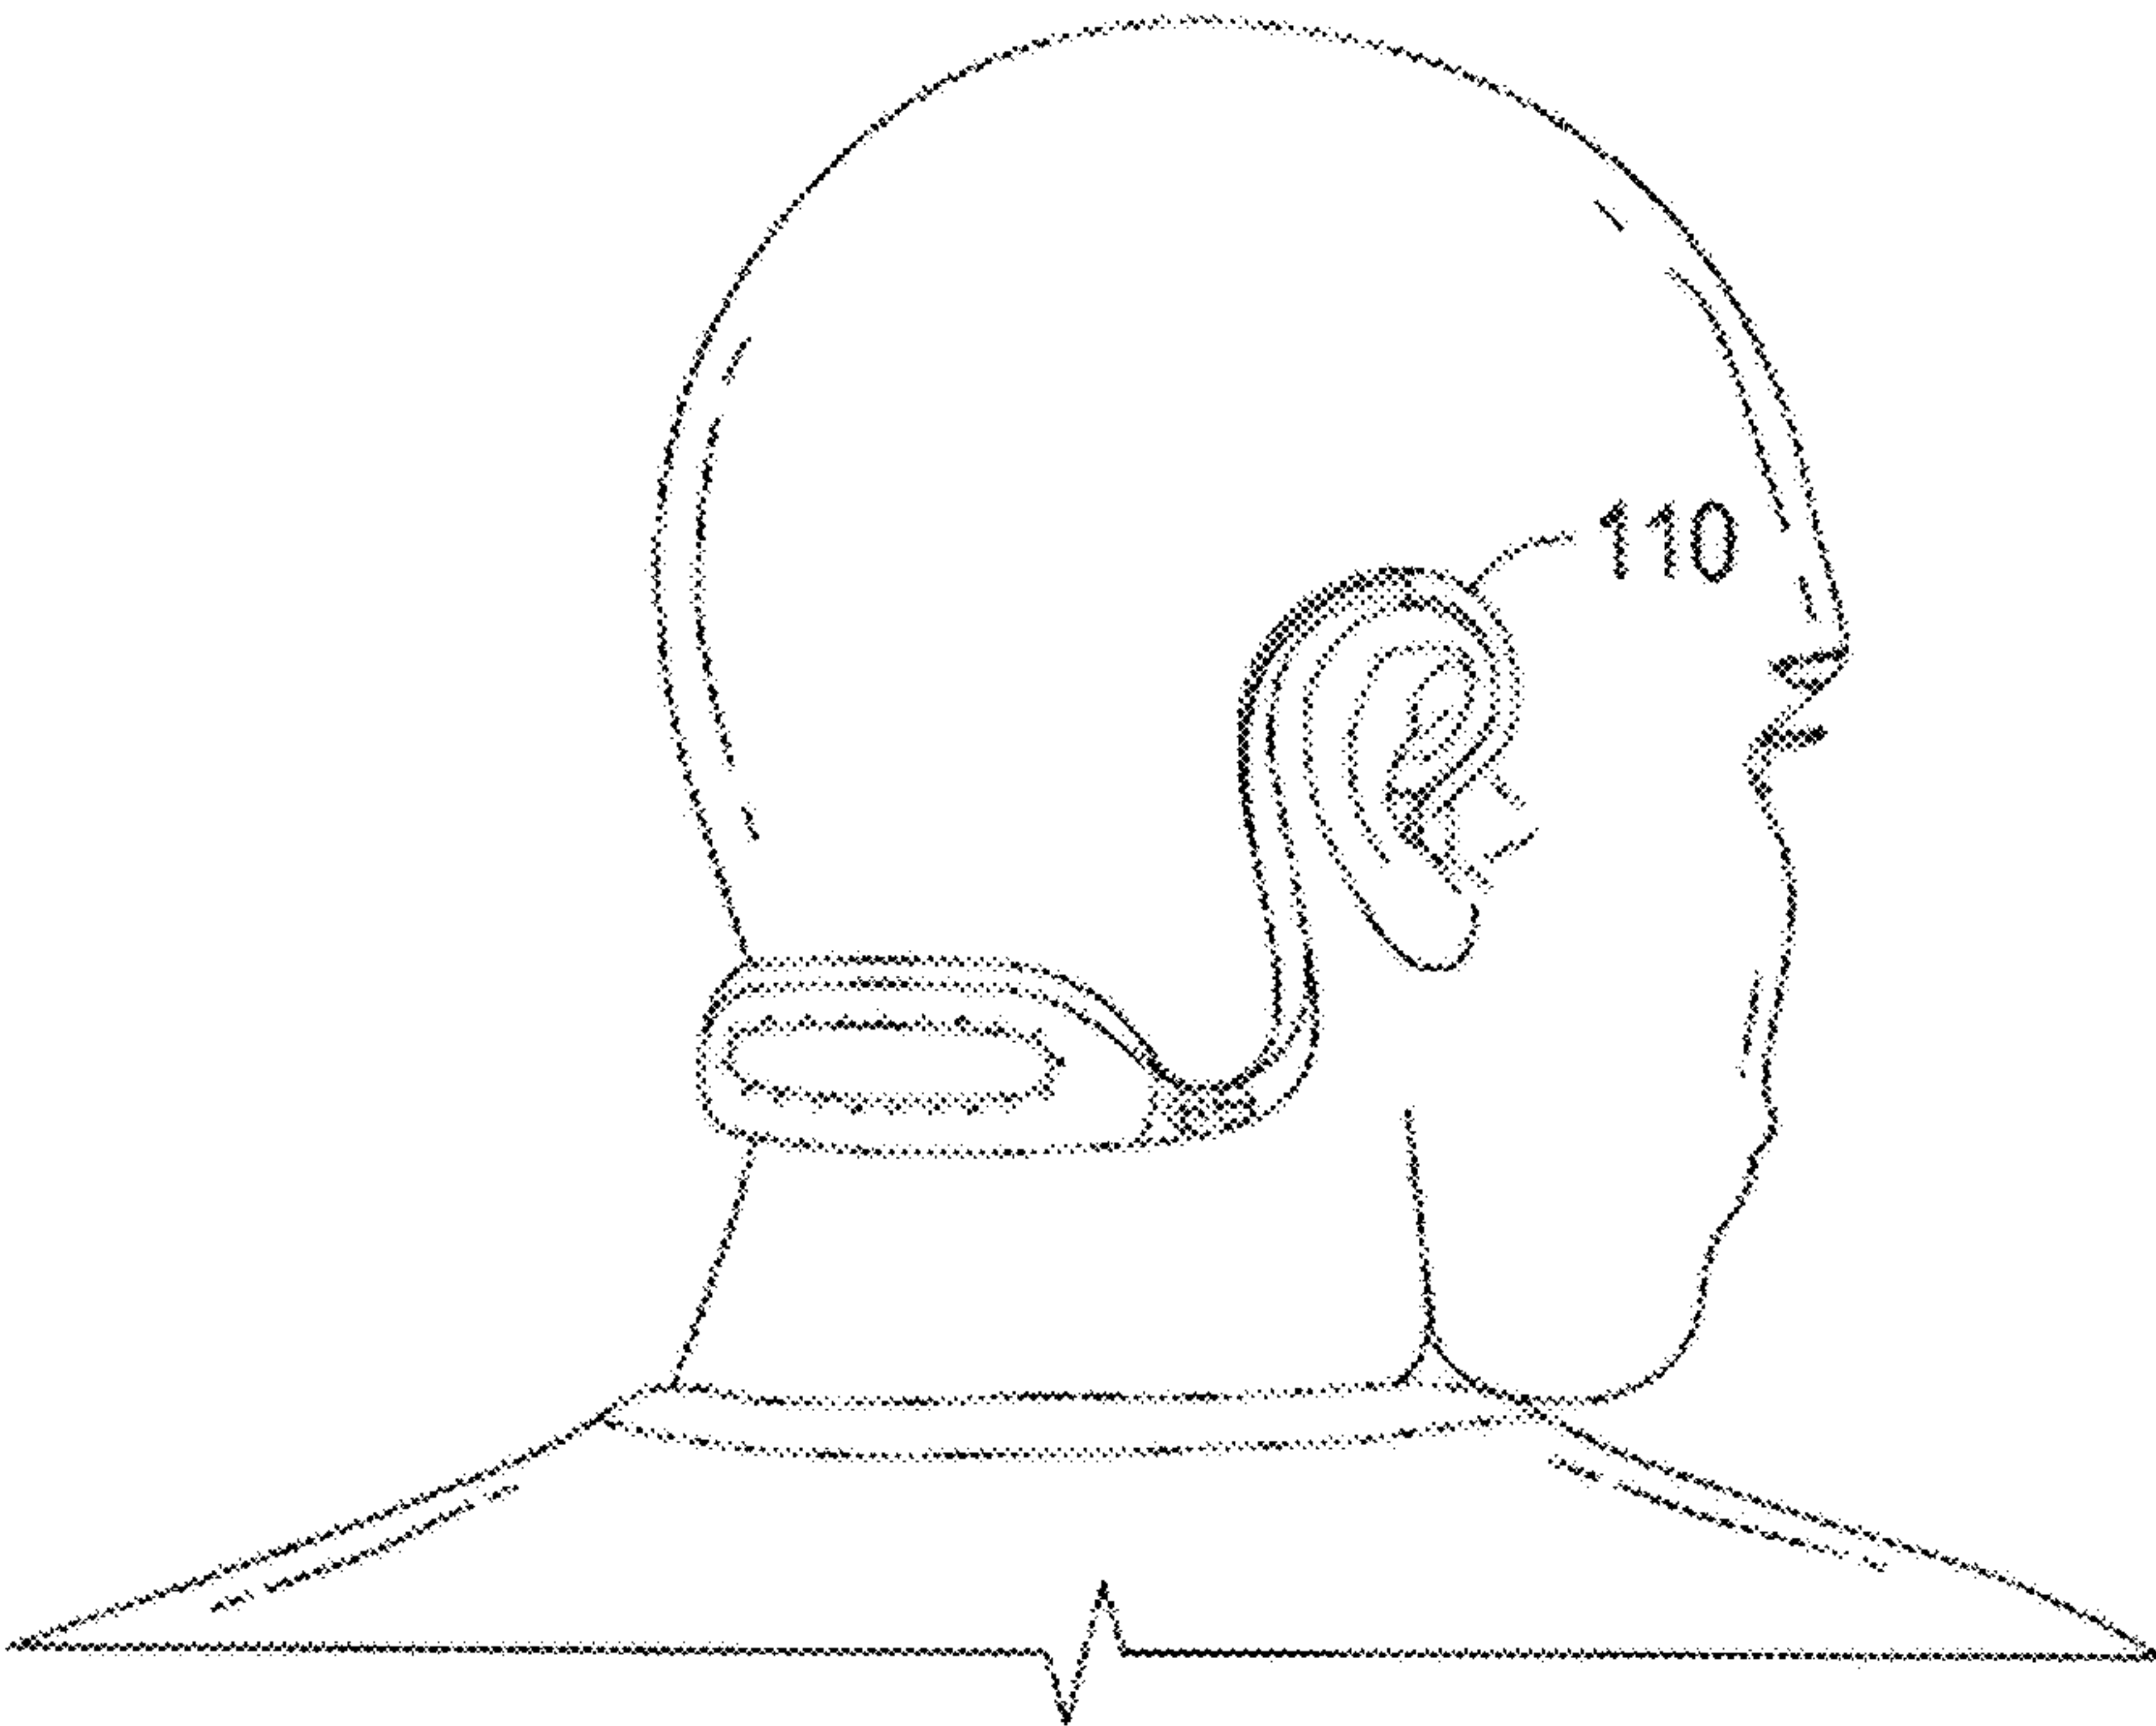
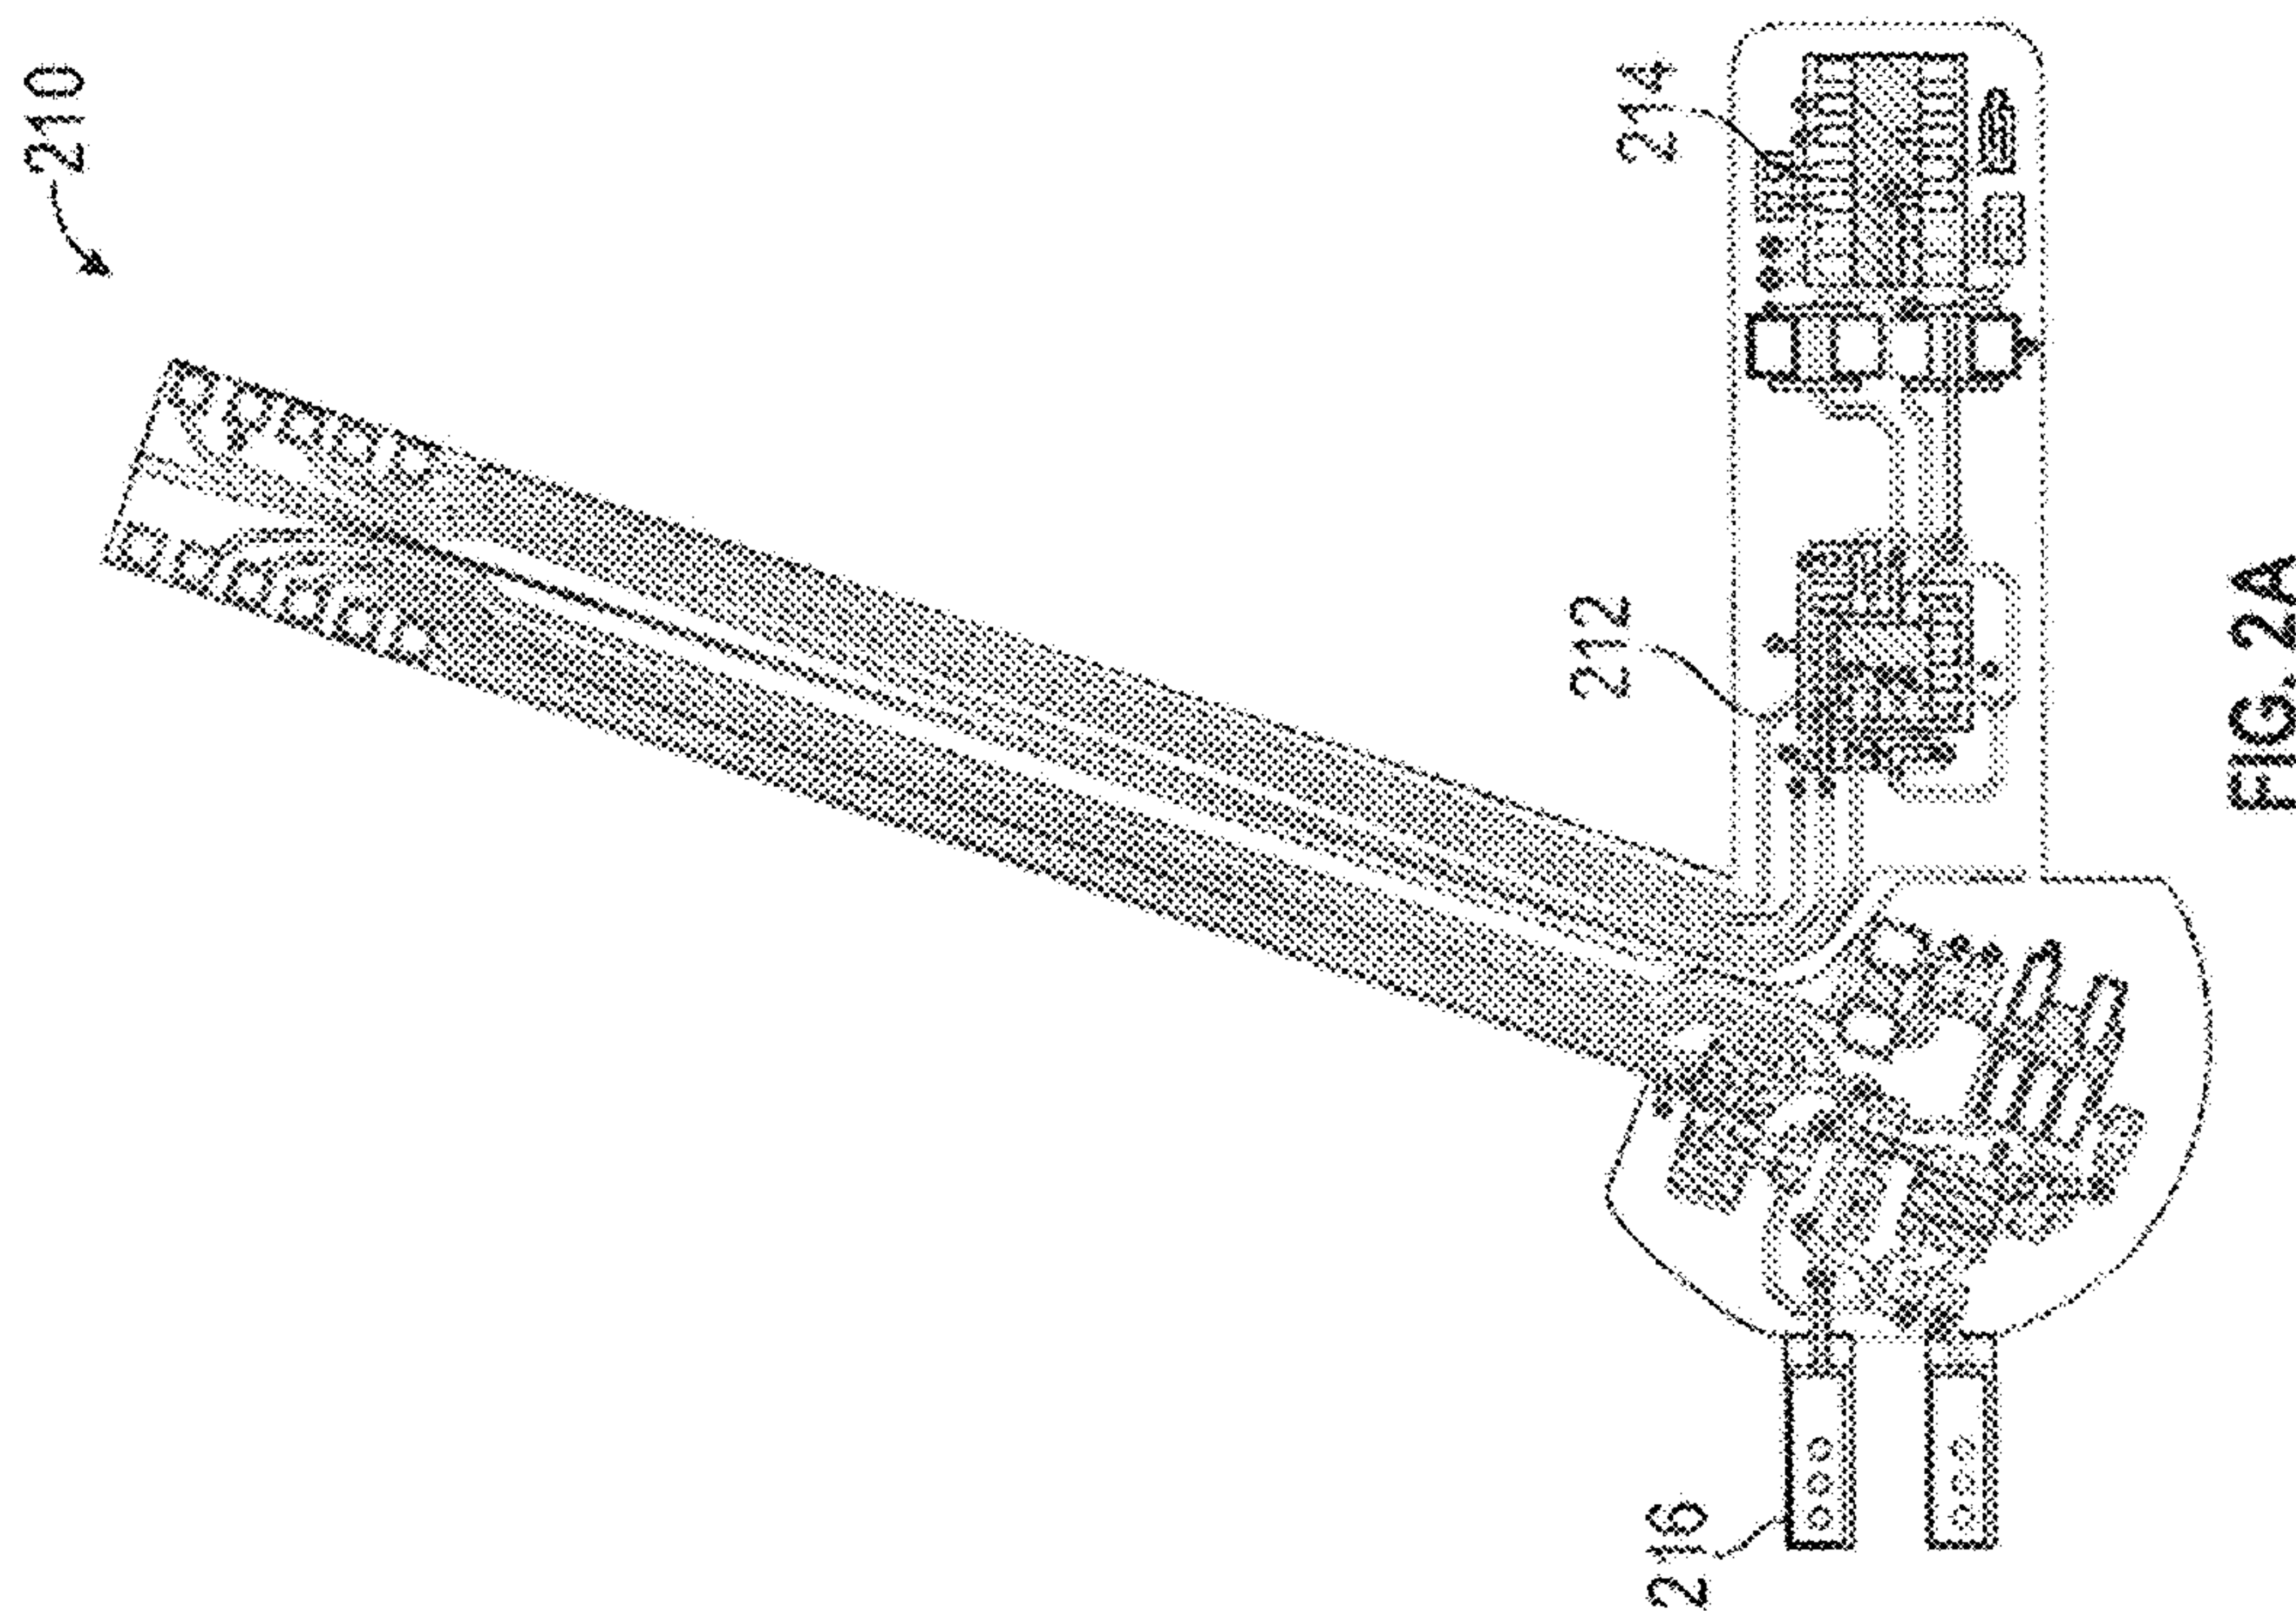
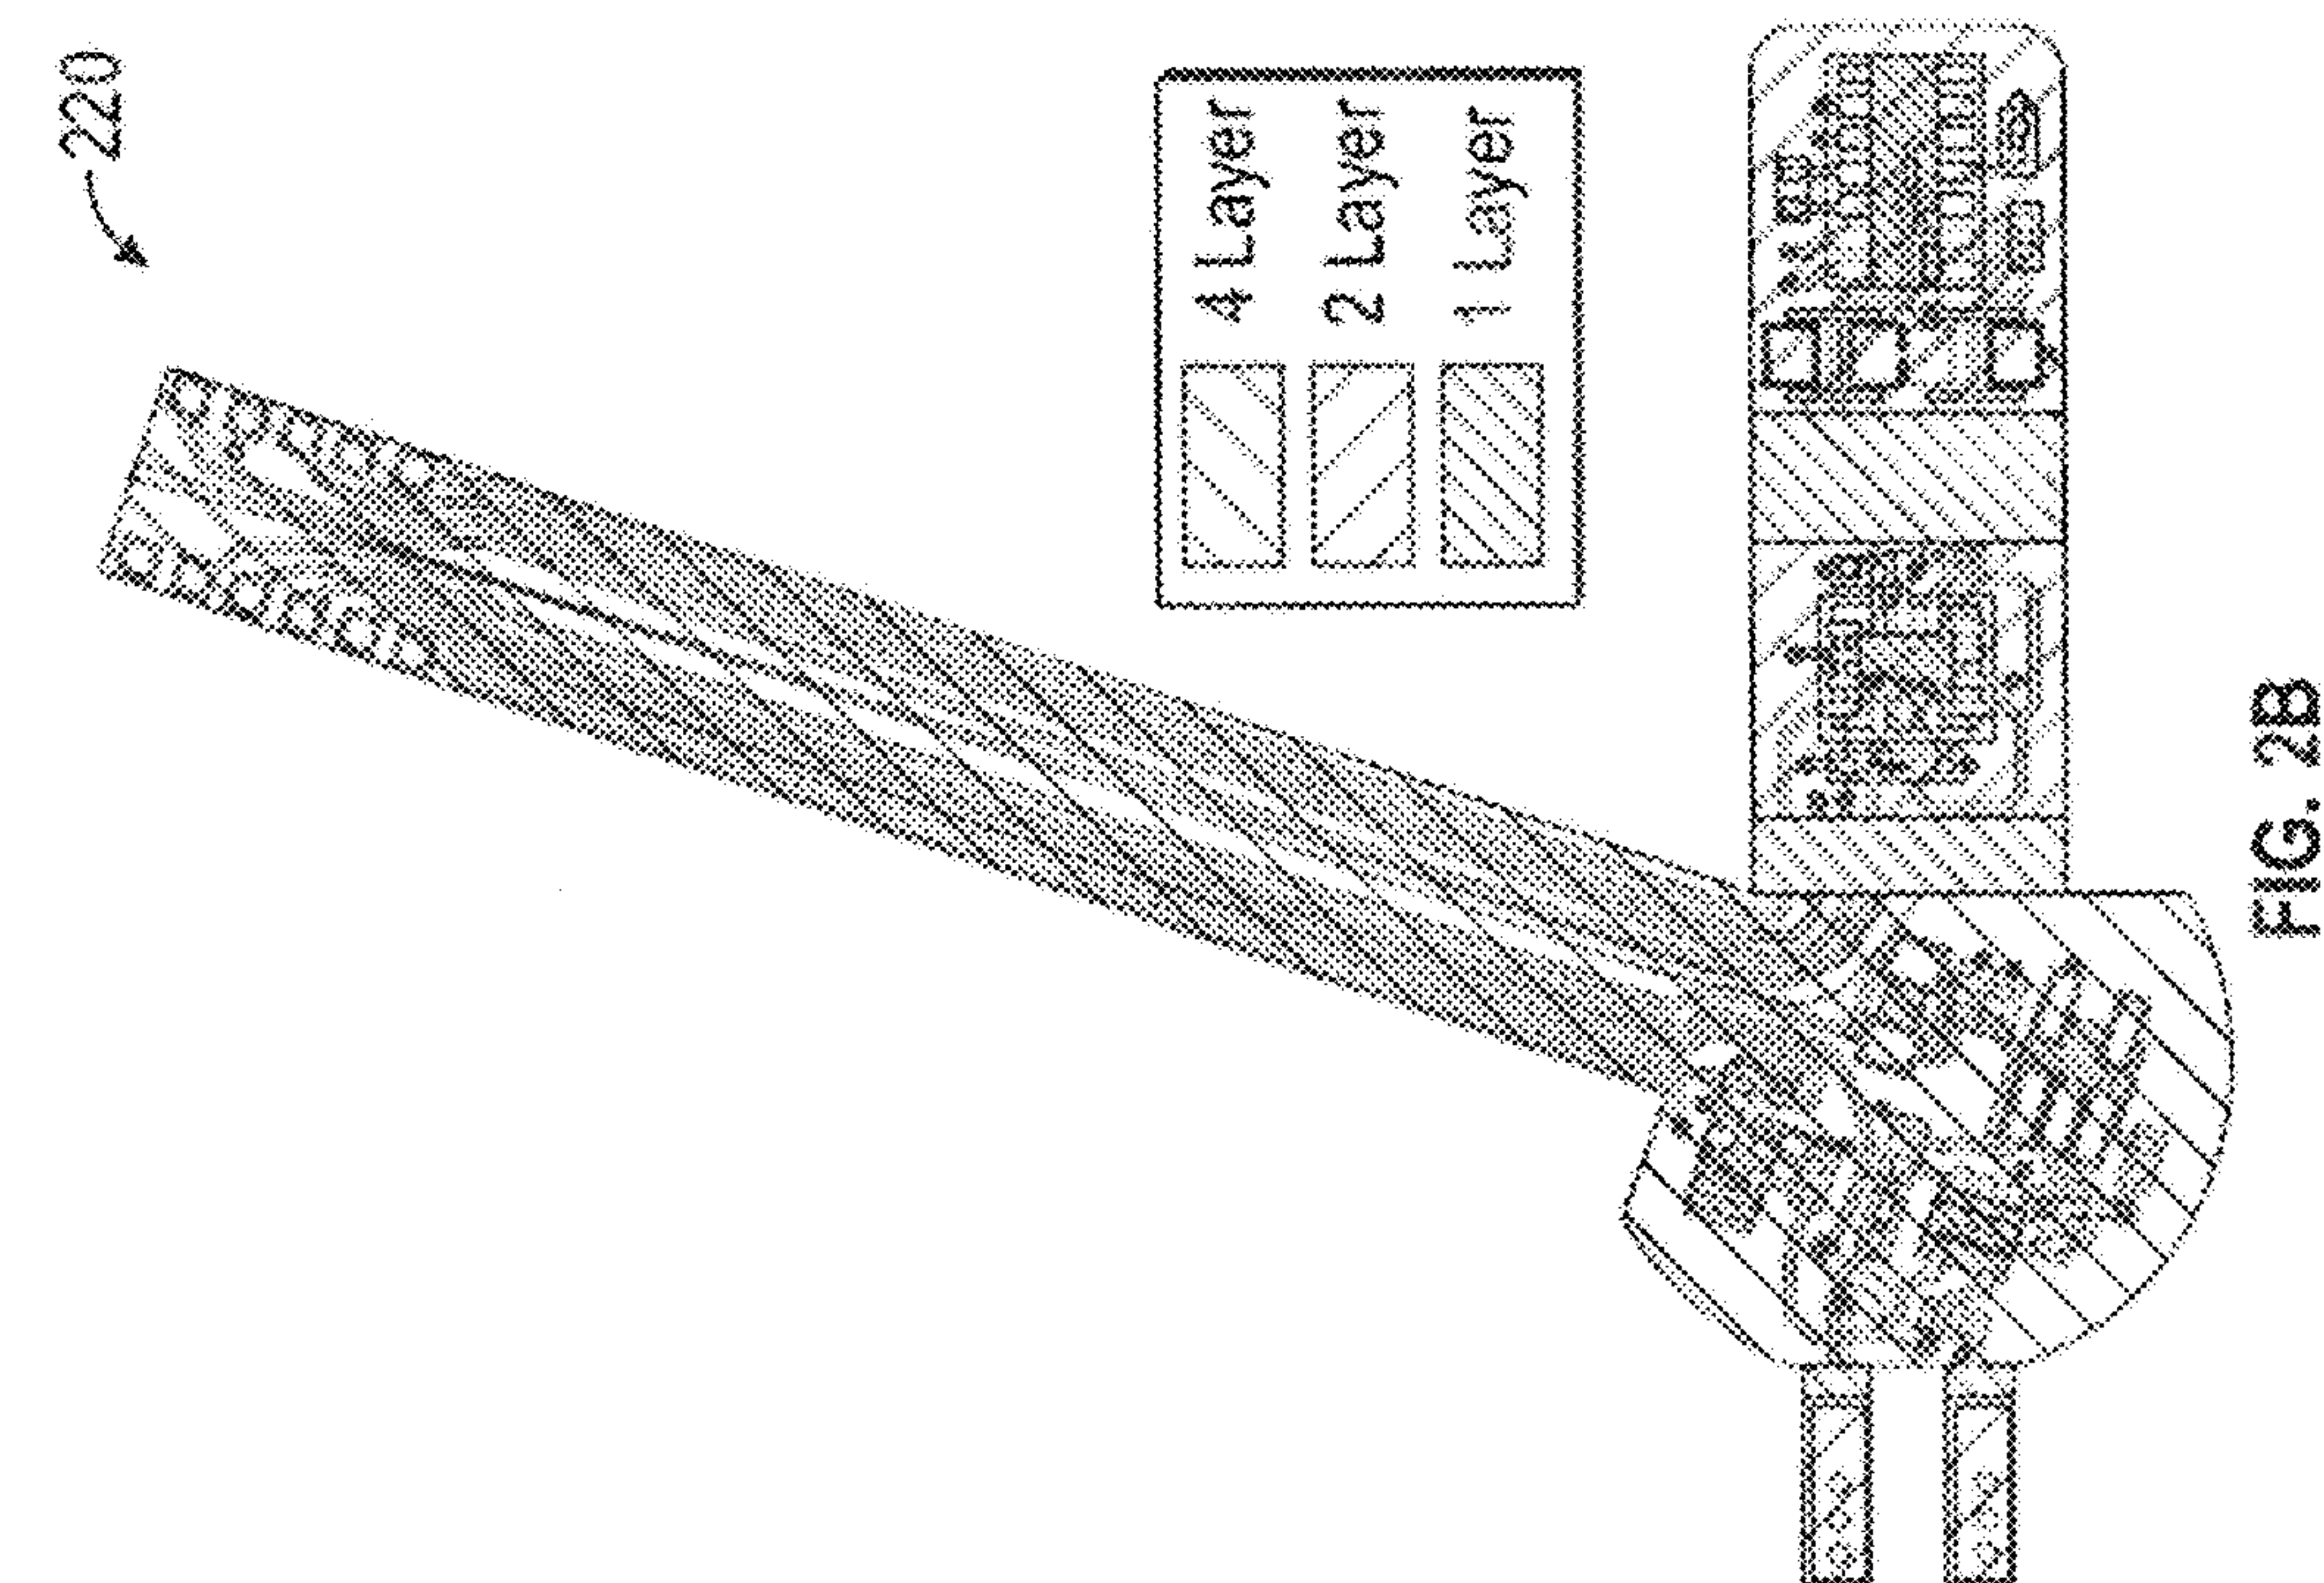


FIG. 1B



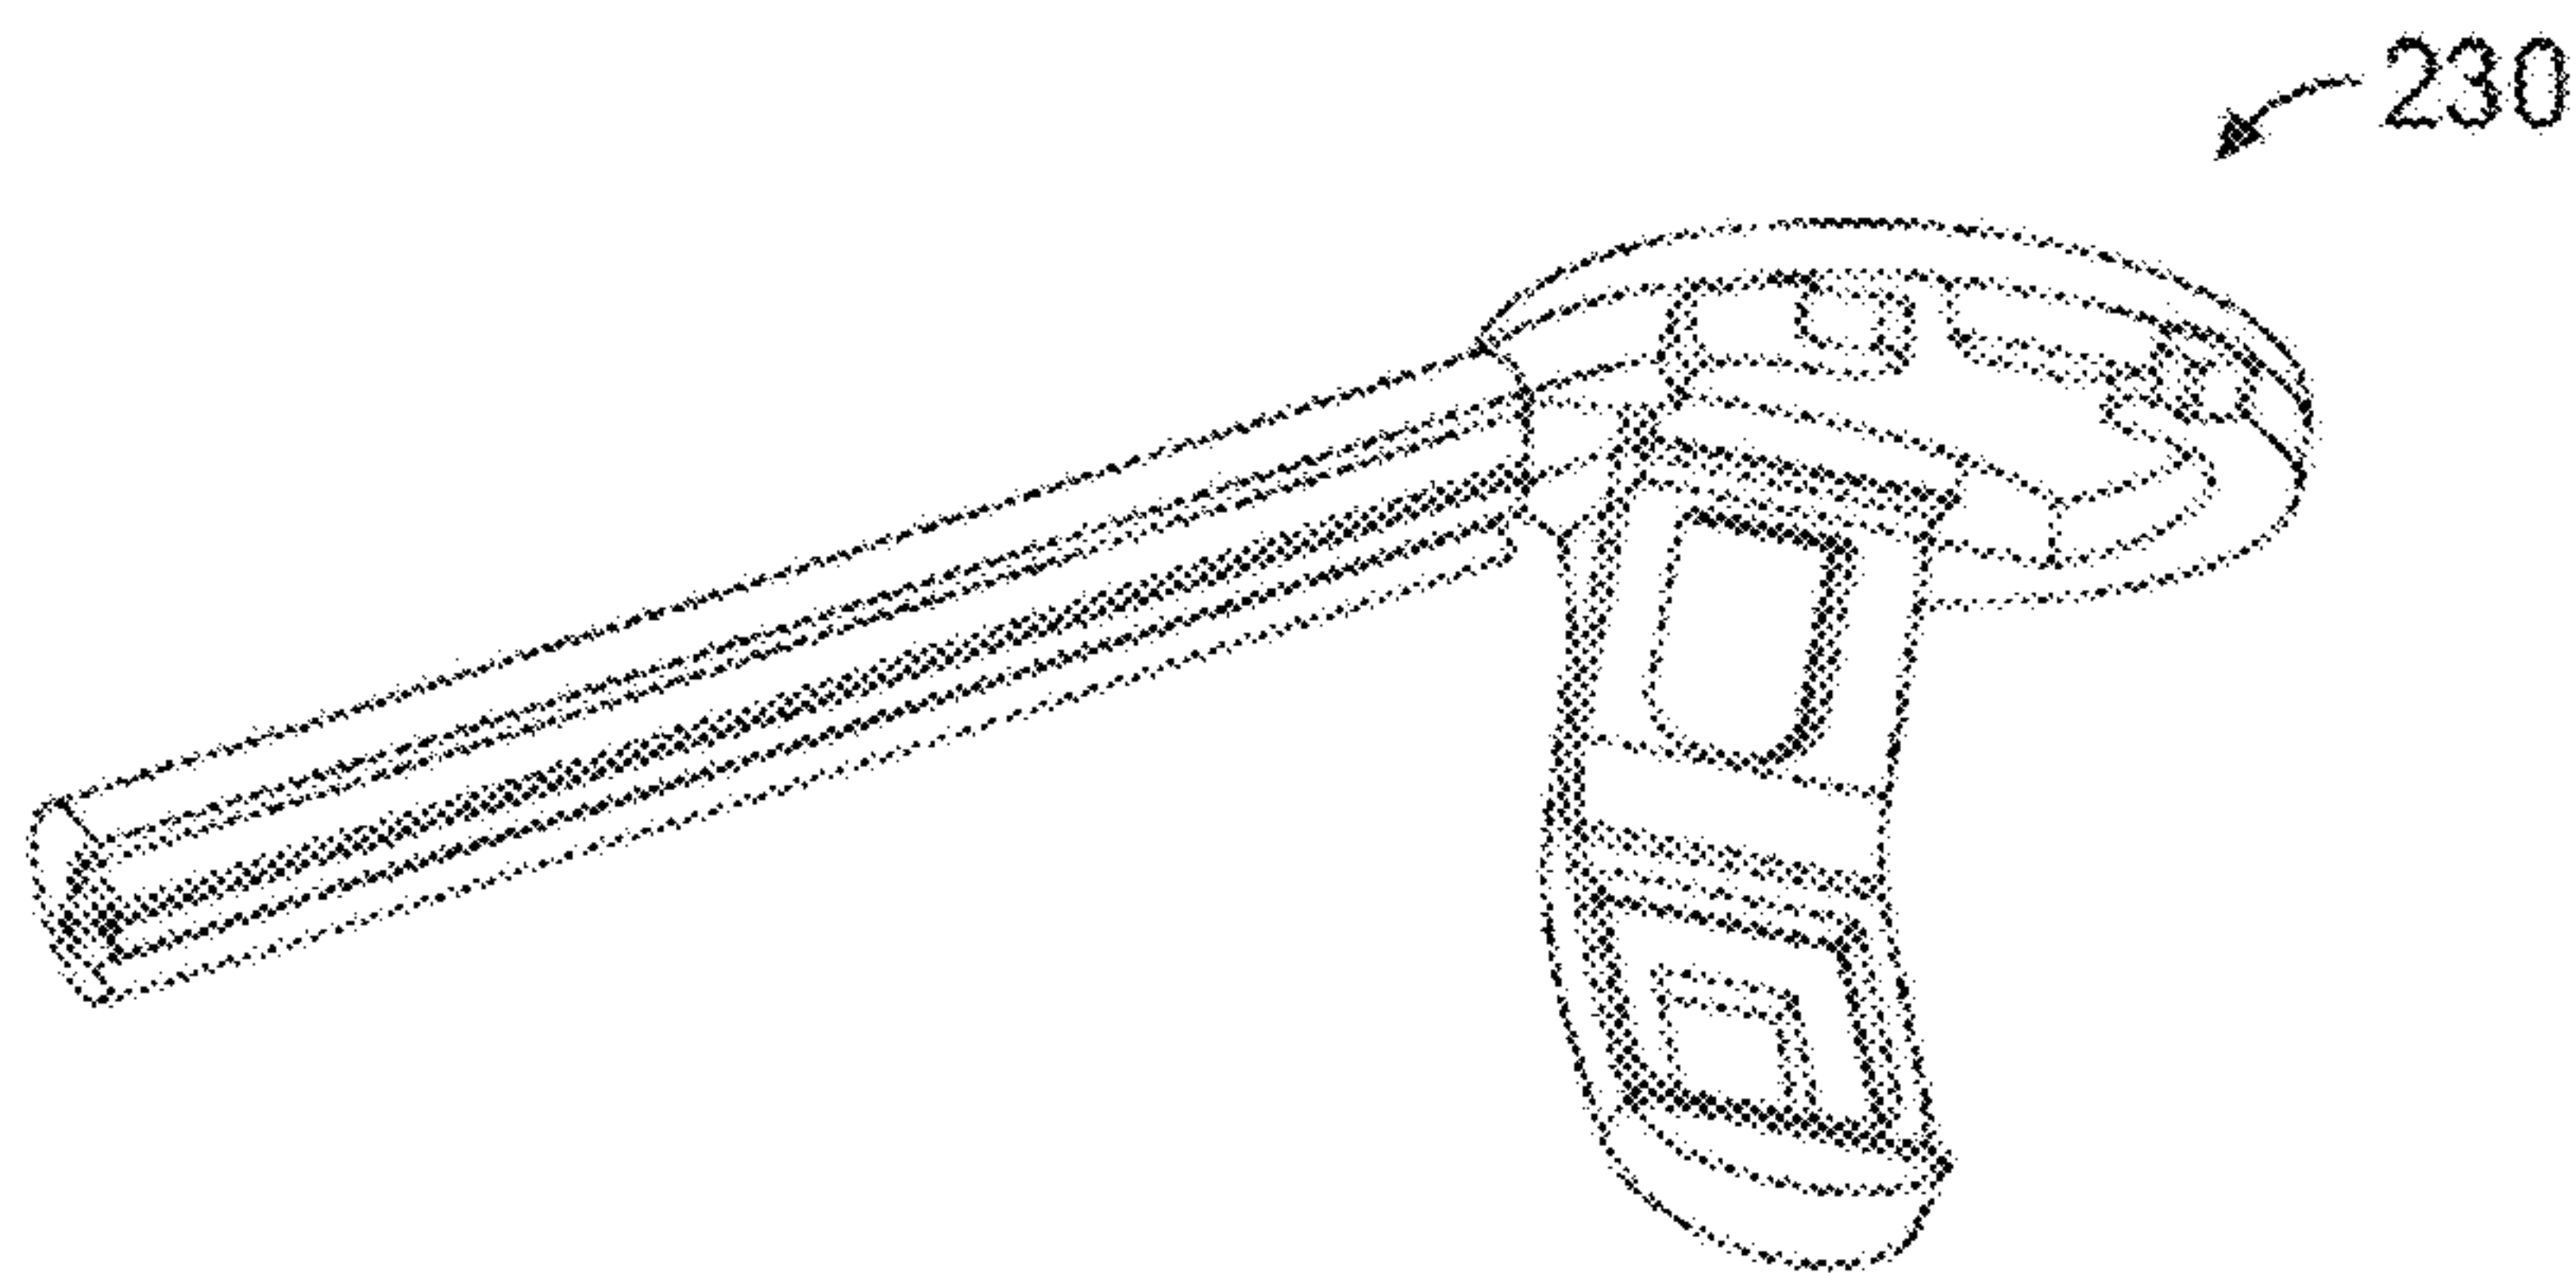


FIG. 2C

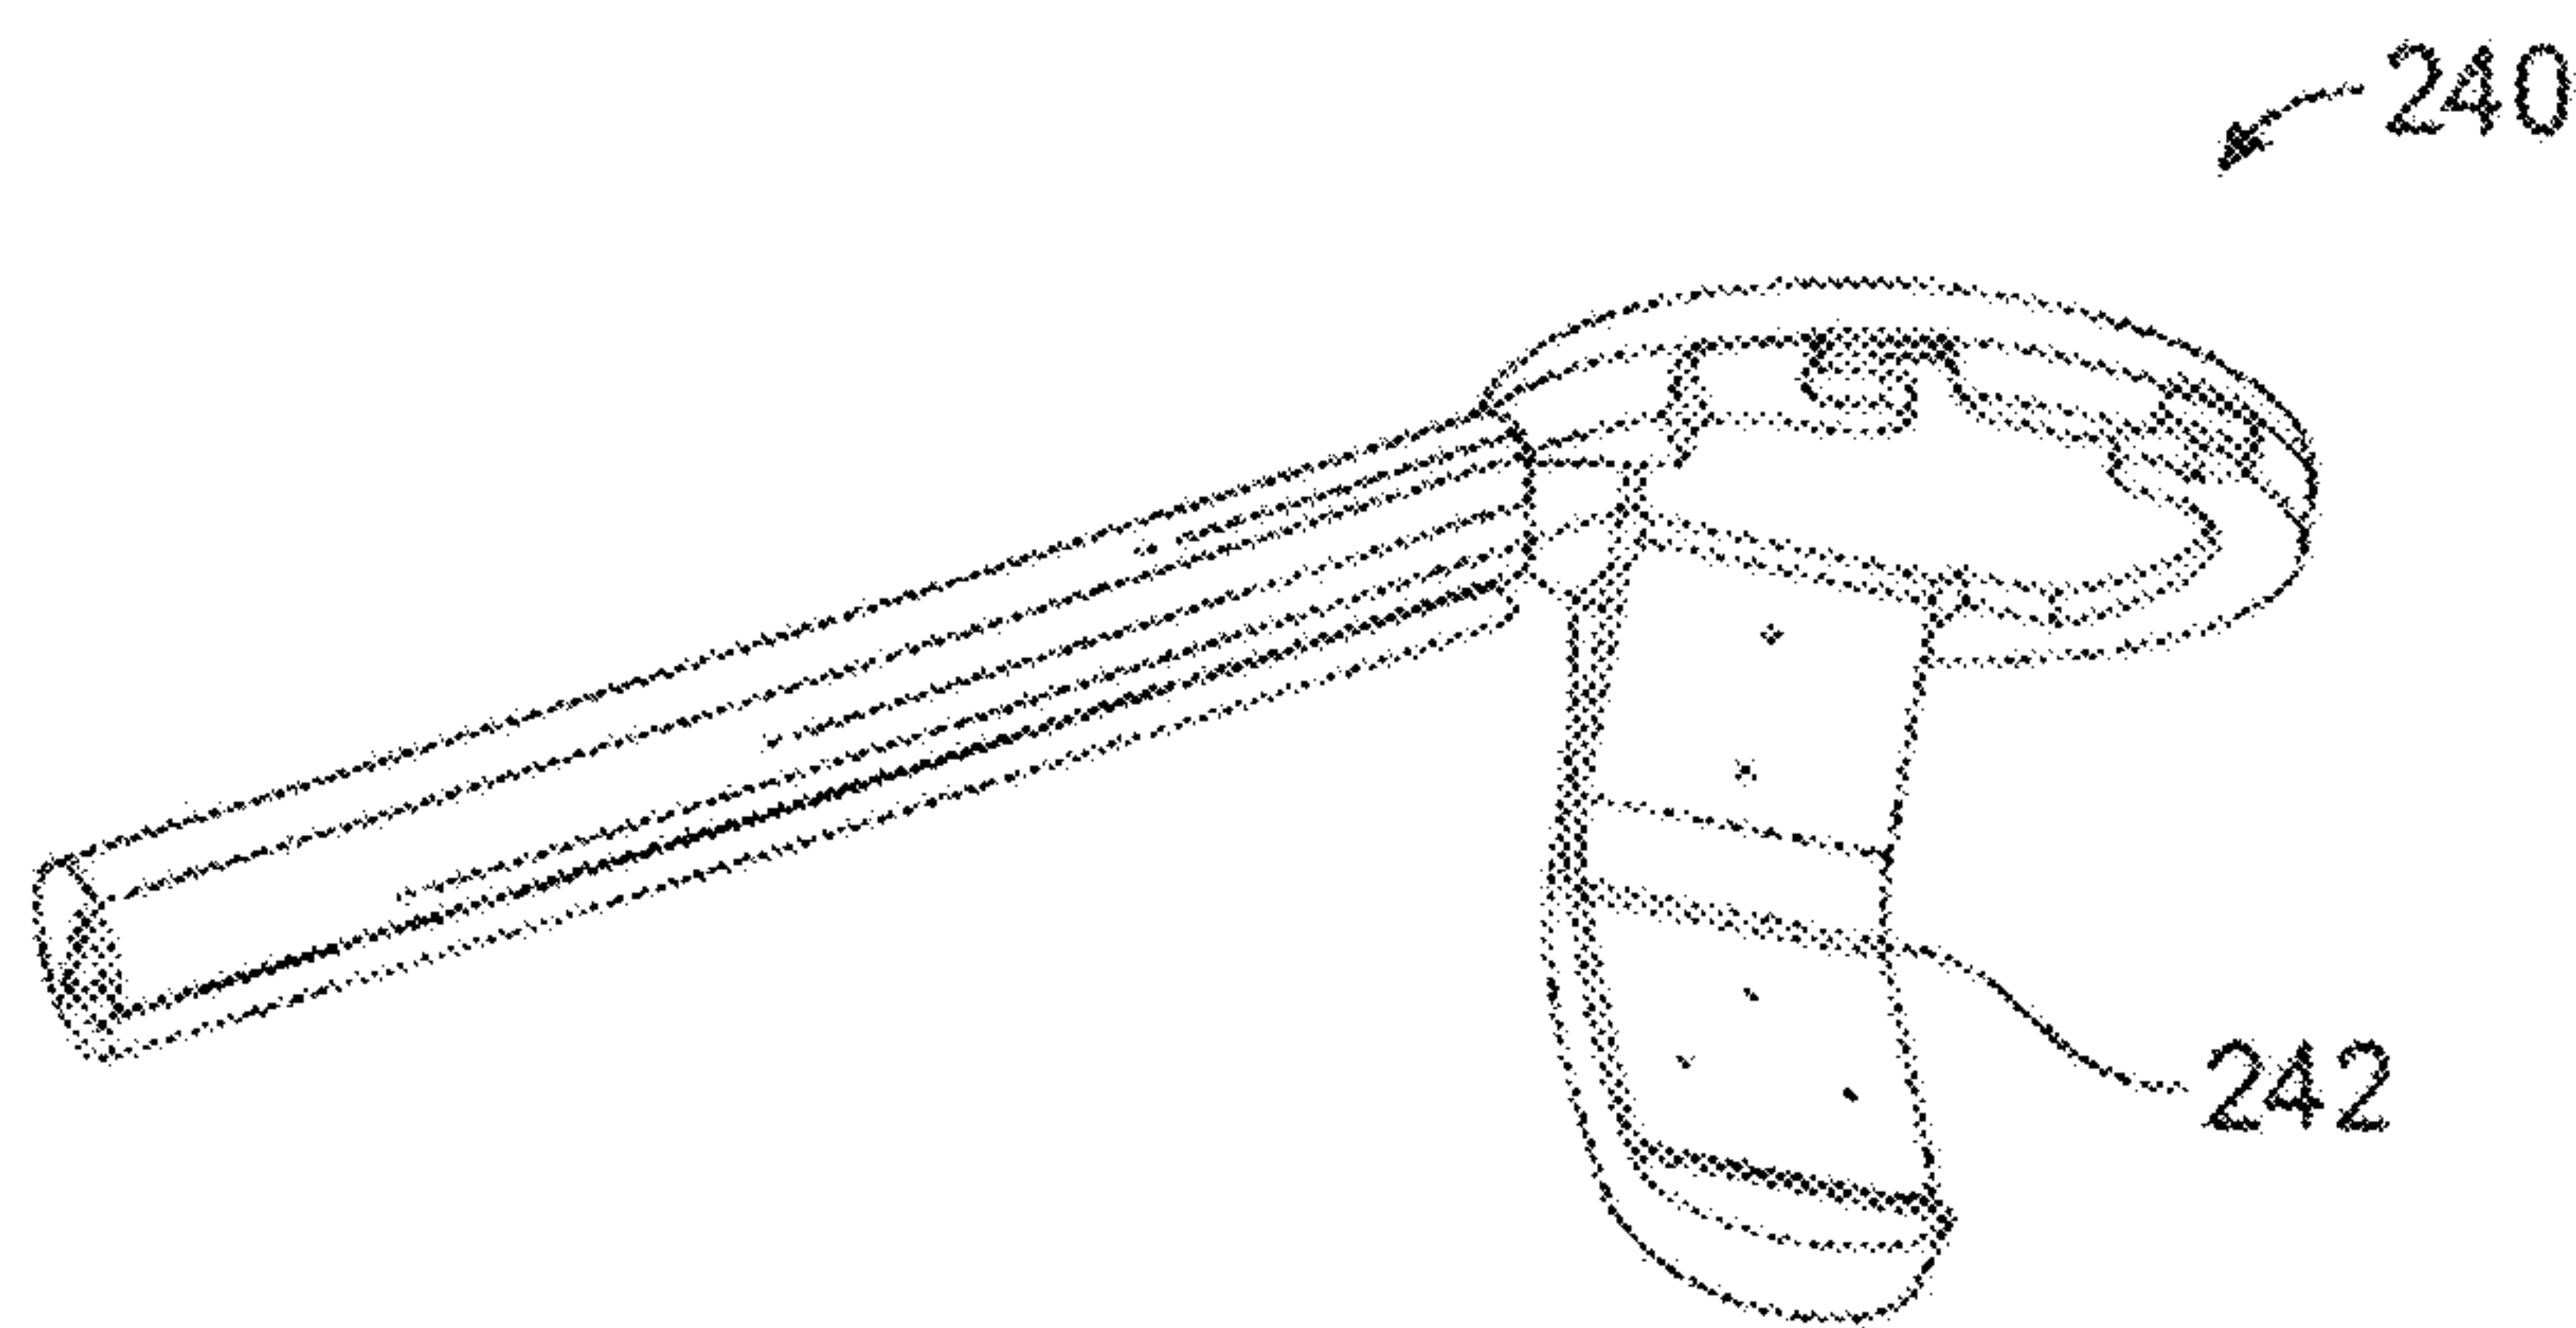


FIG. 2D

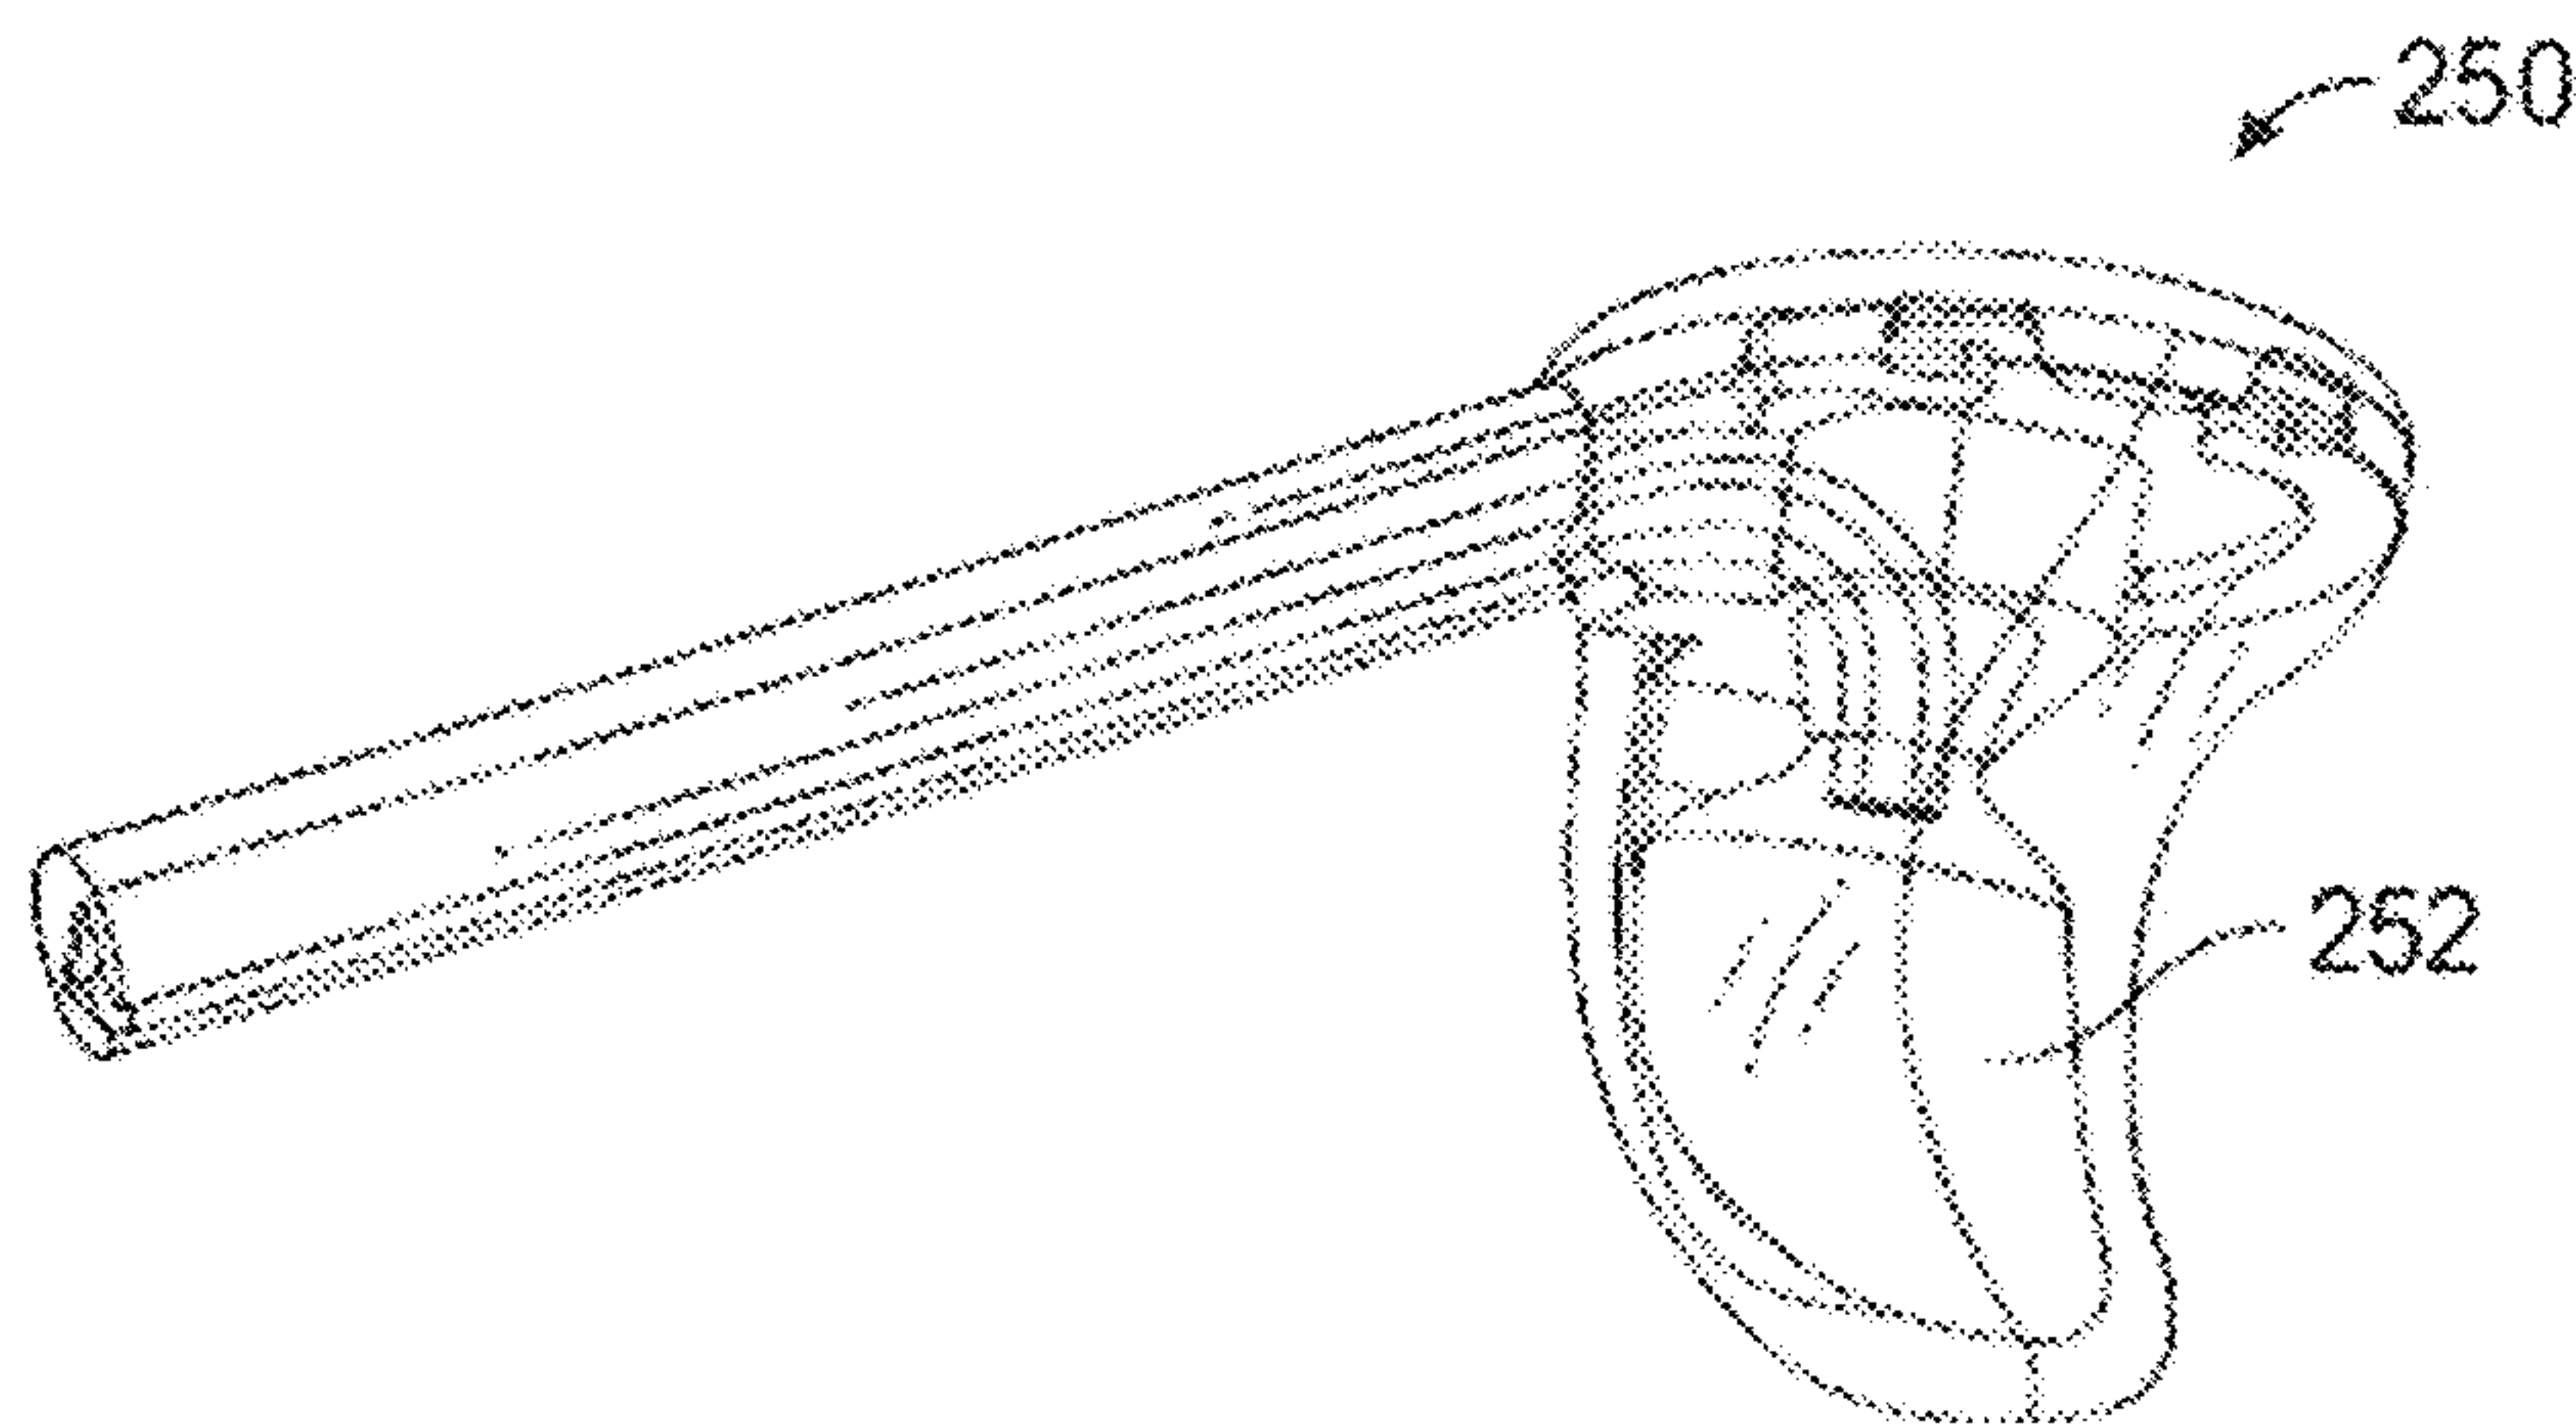


FIG. 2E

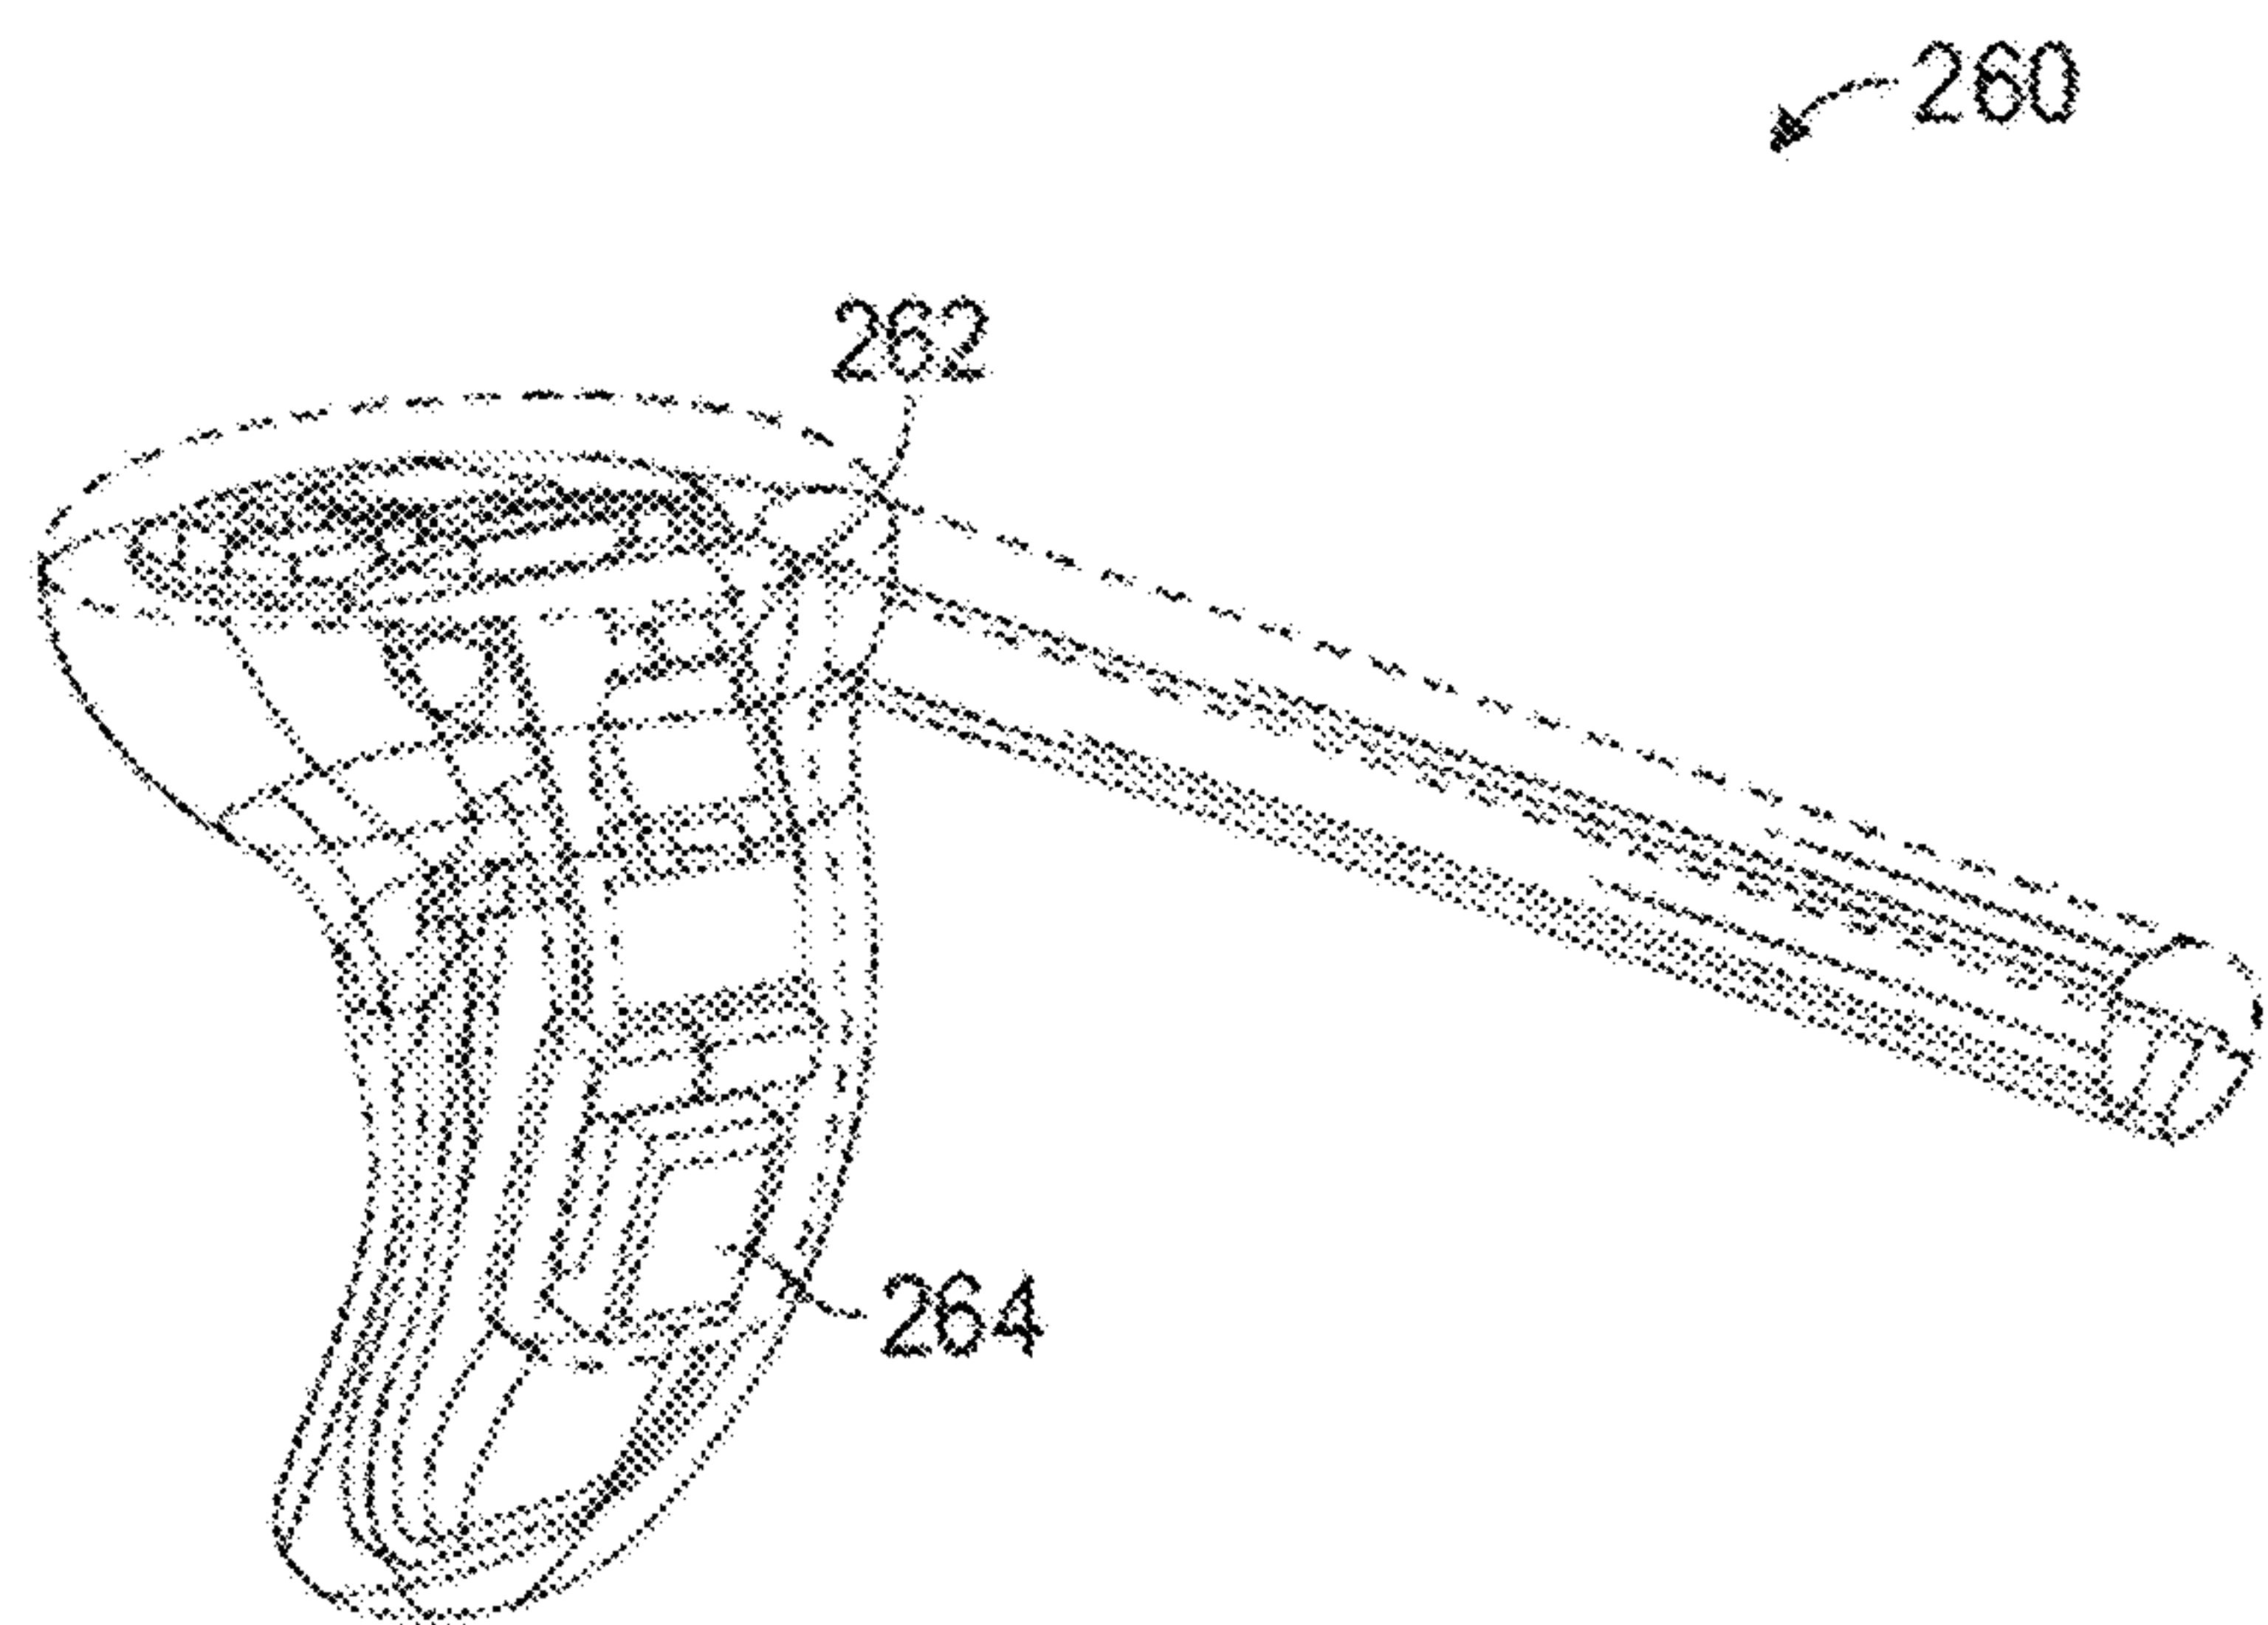


FIG. 2F

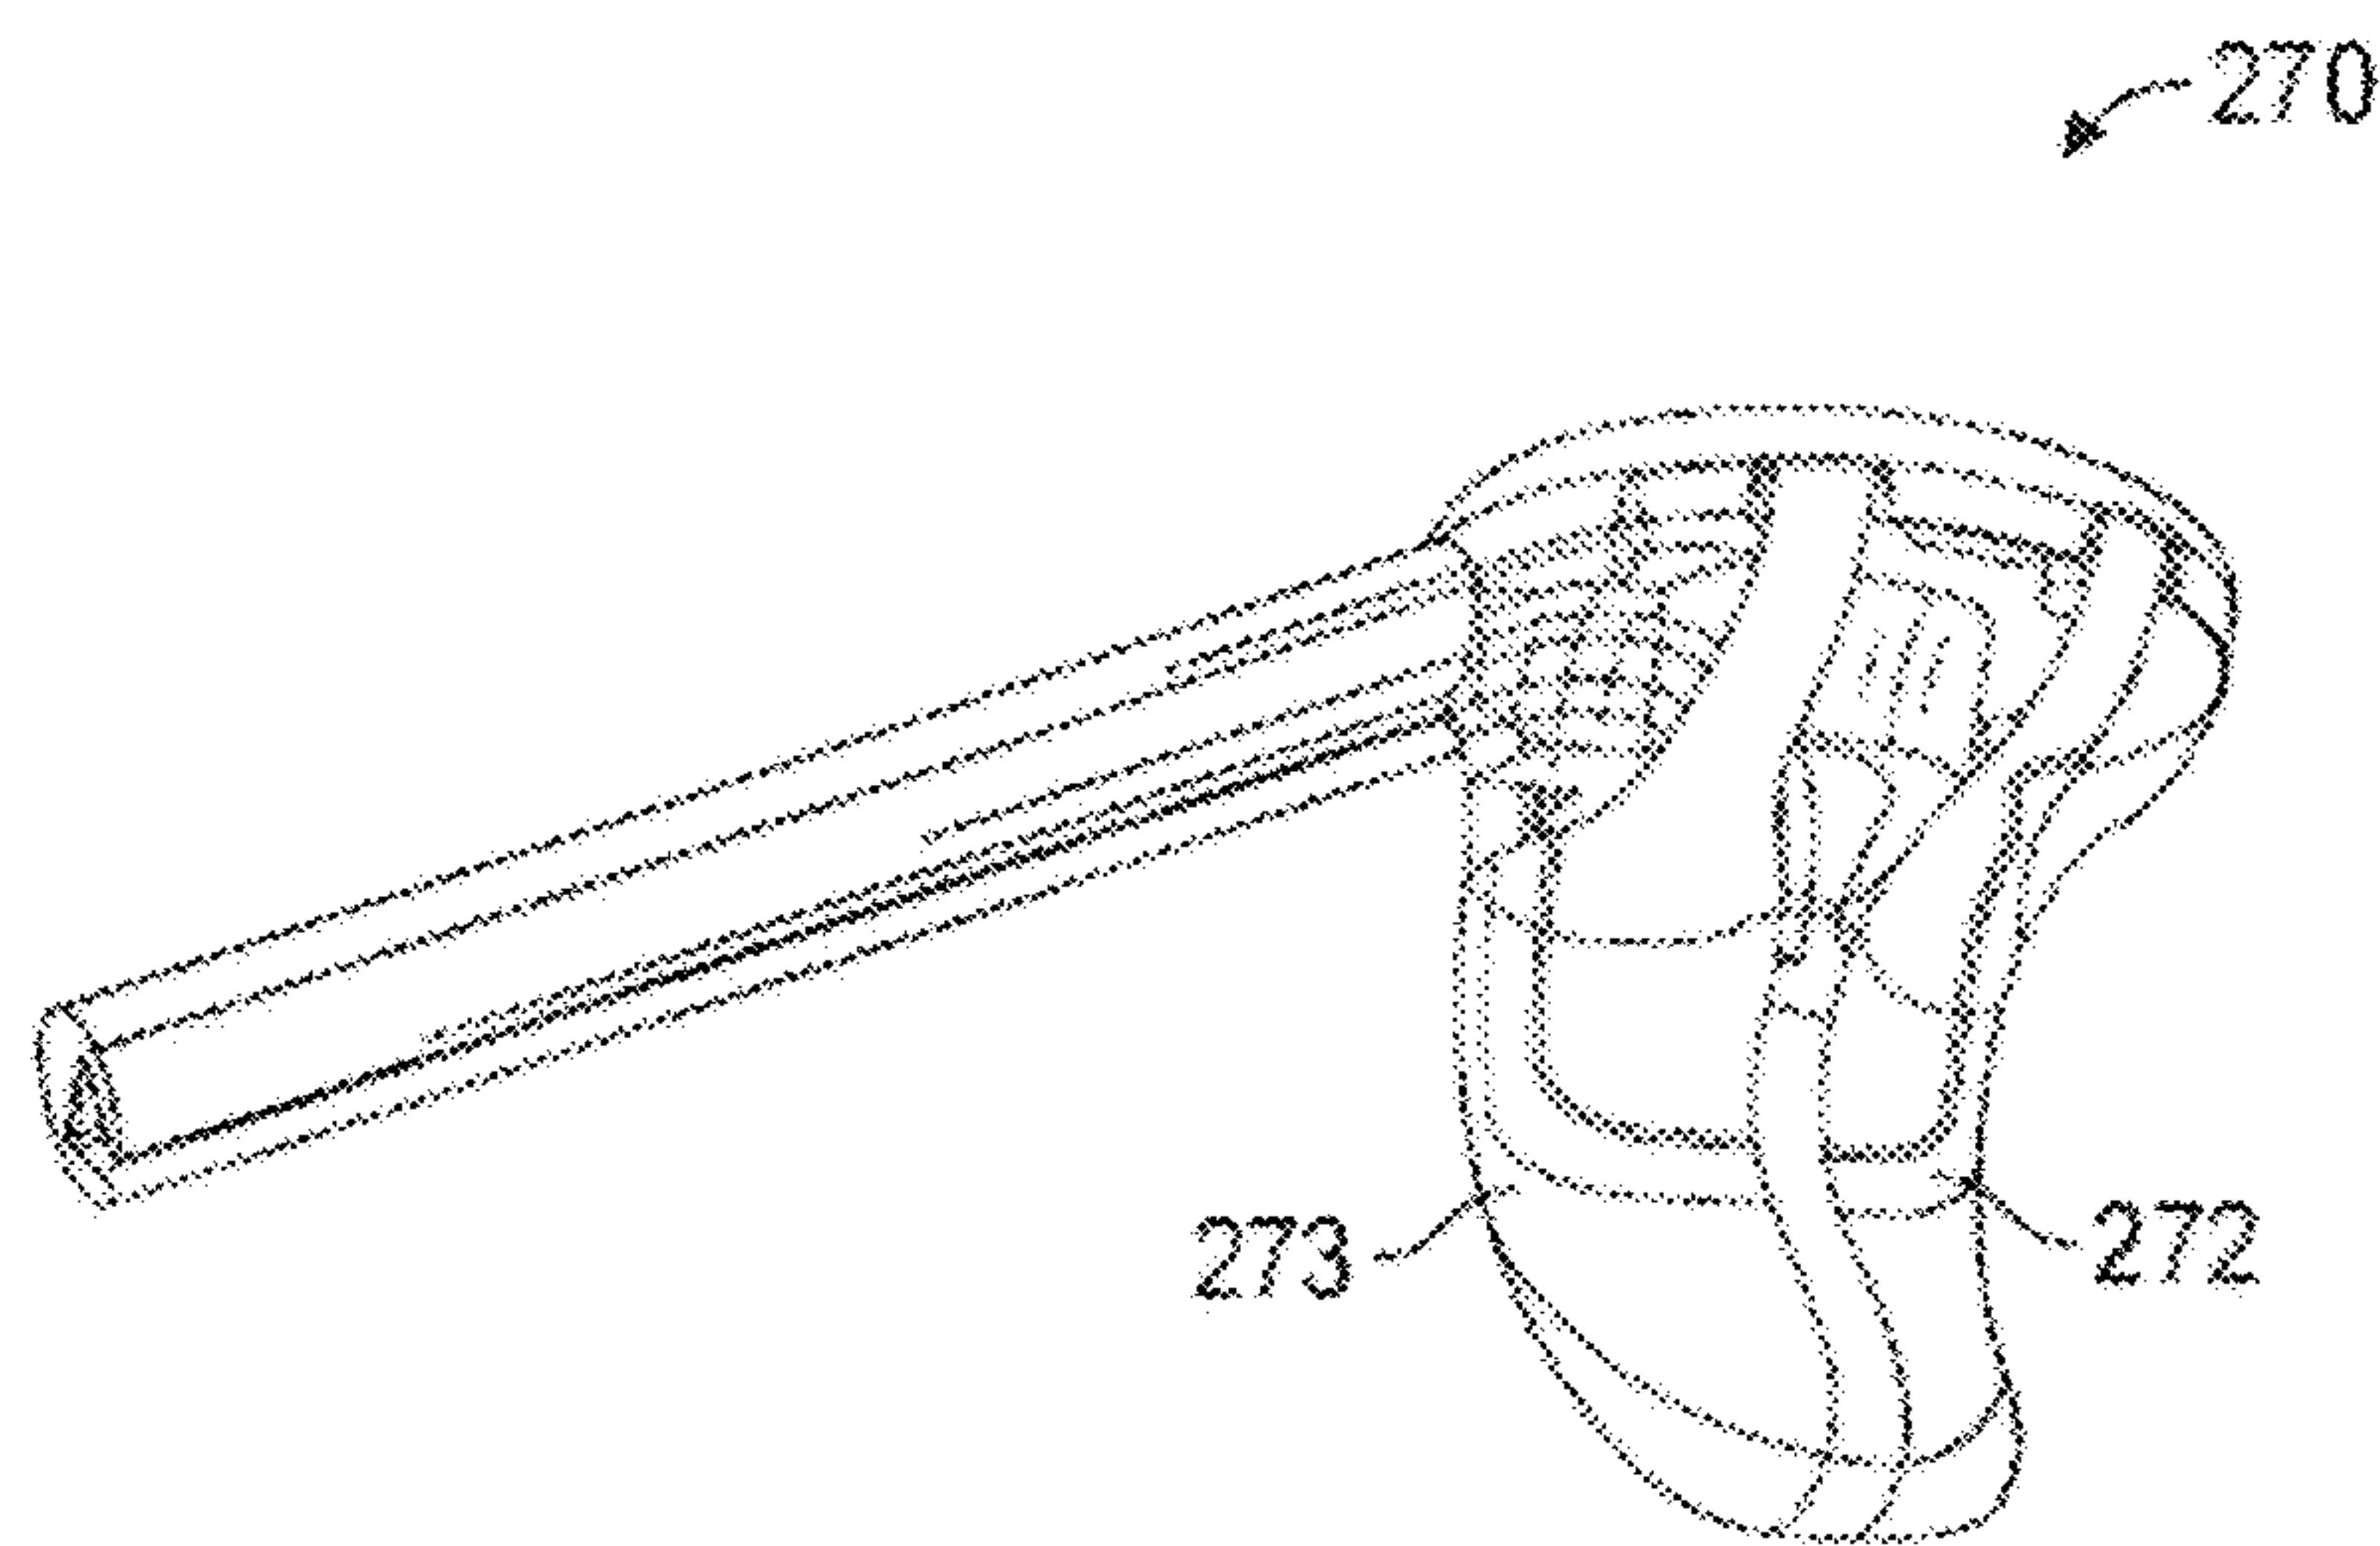


FIG. 2G

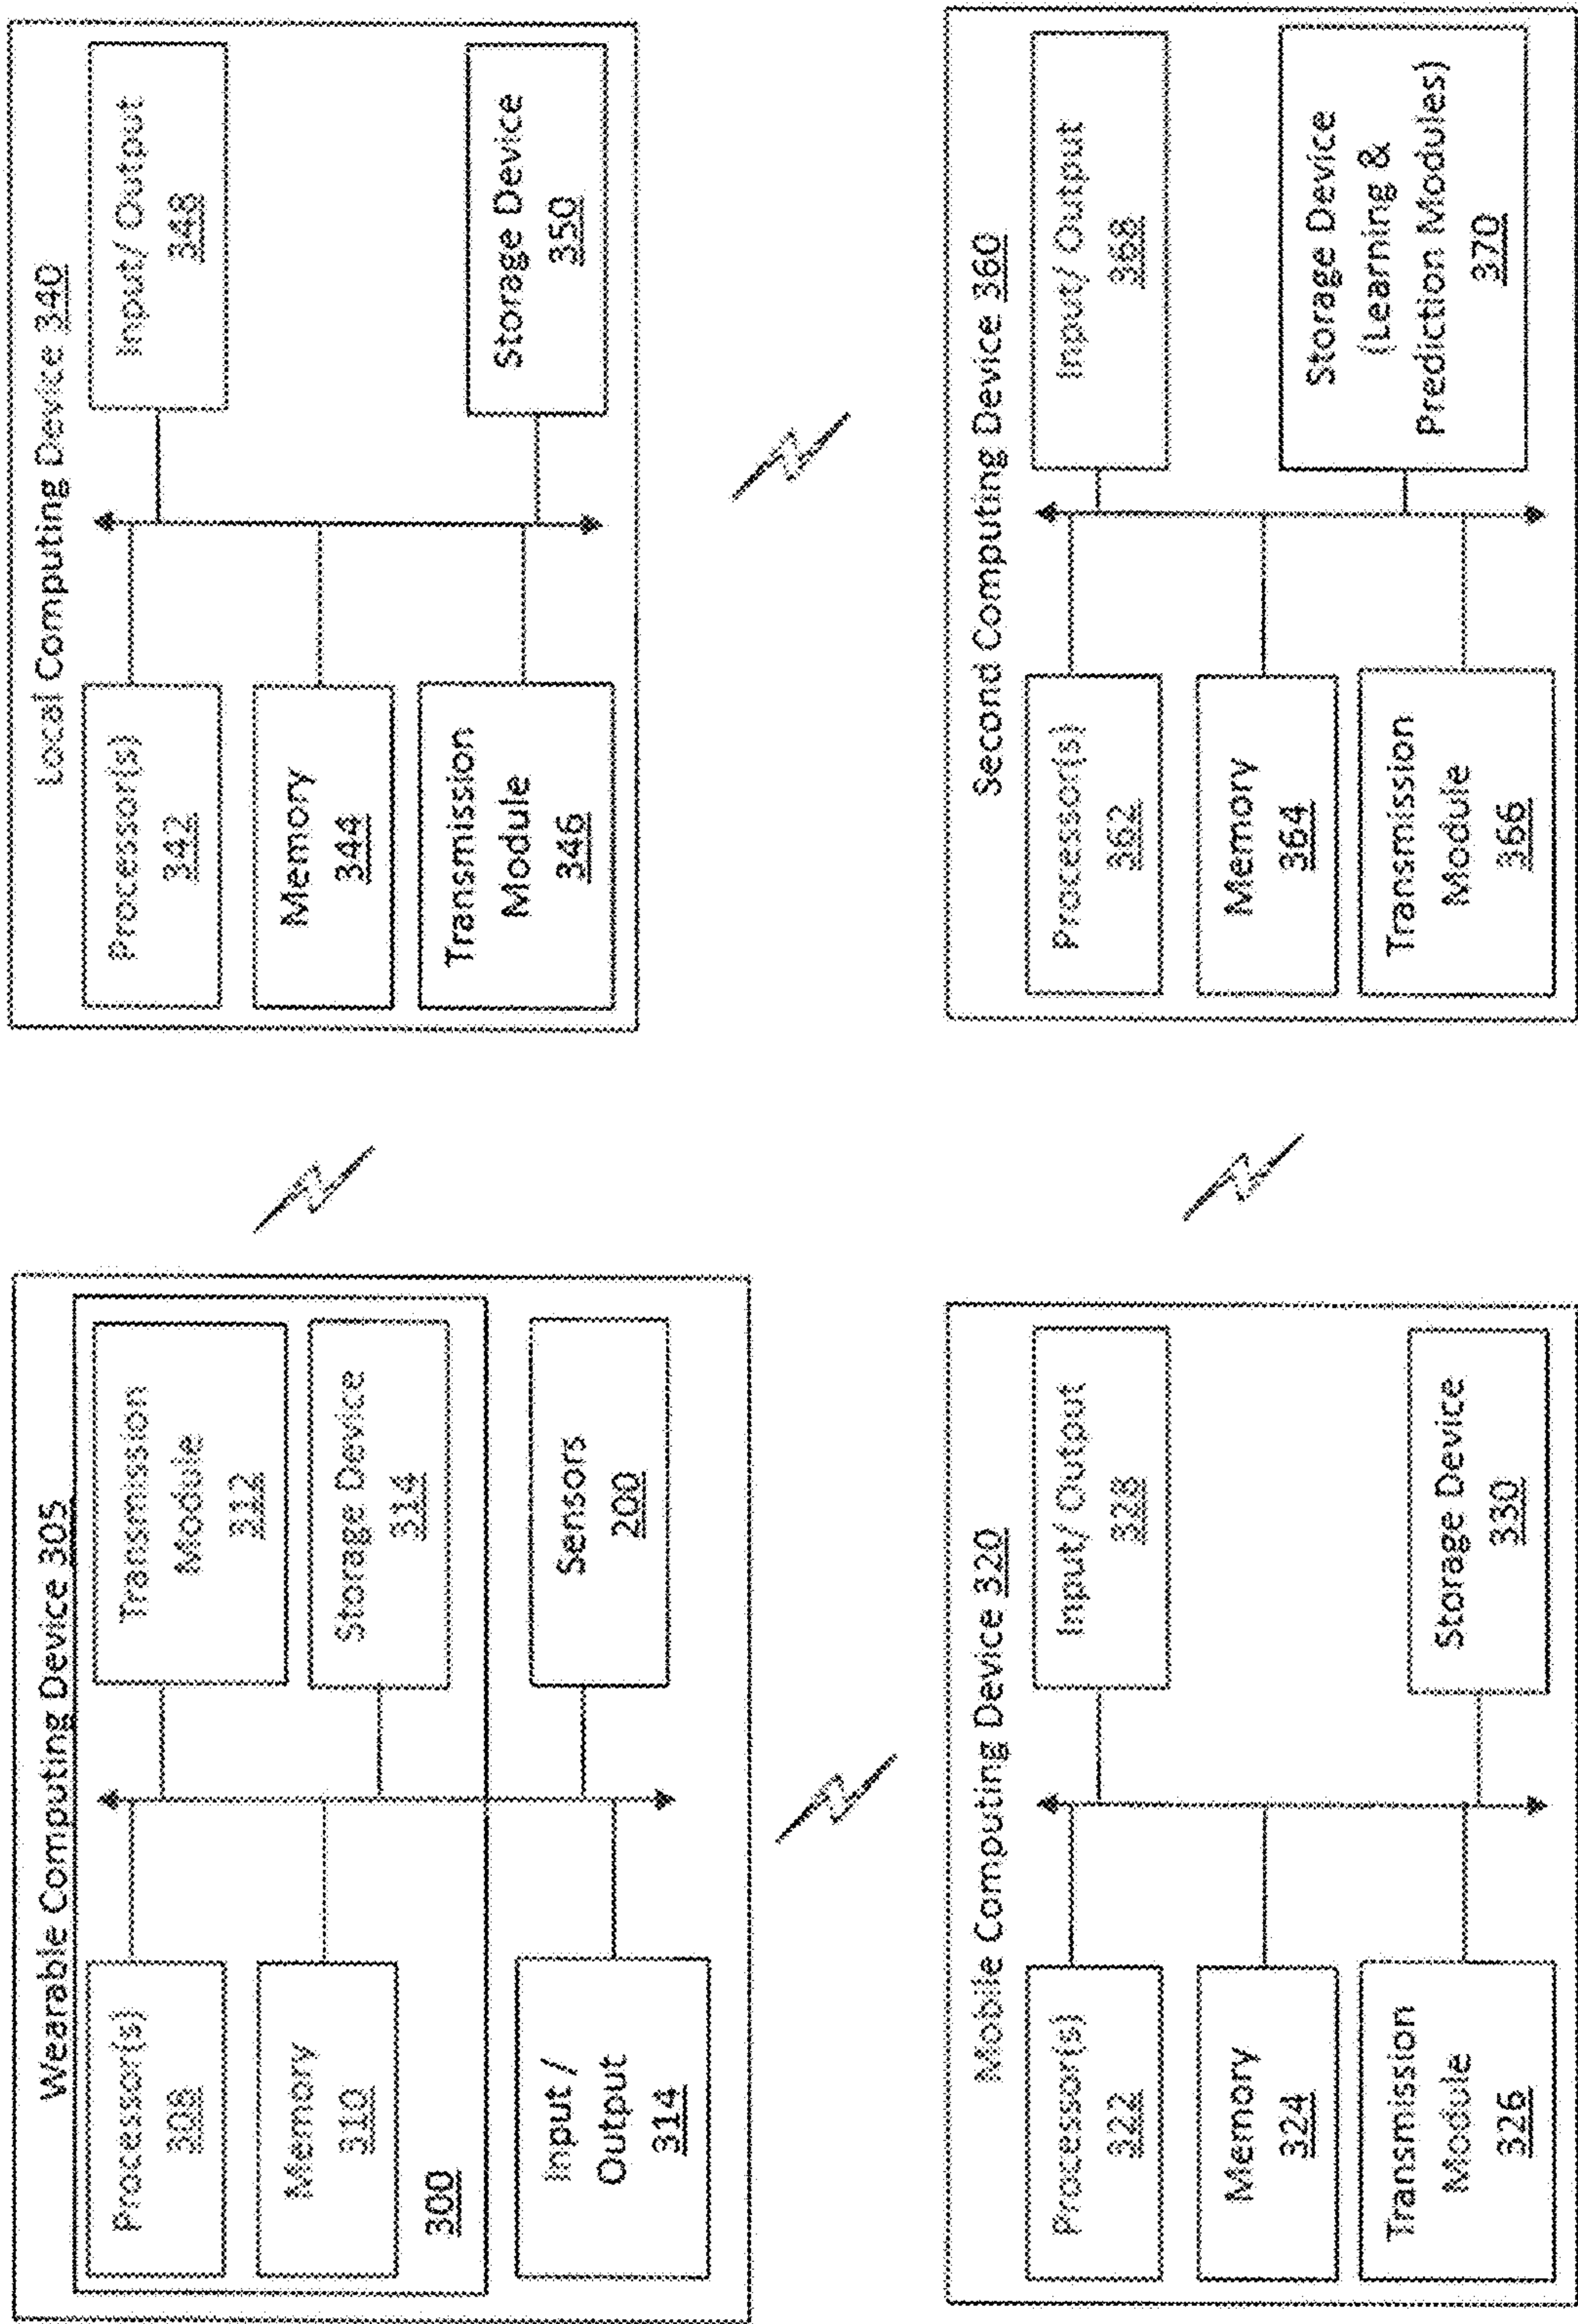


FIG. 3

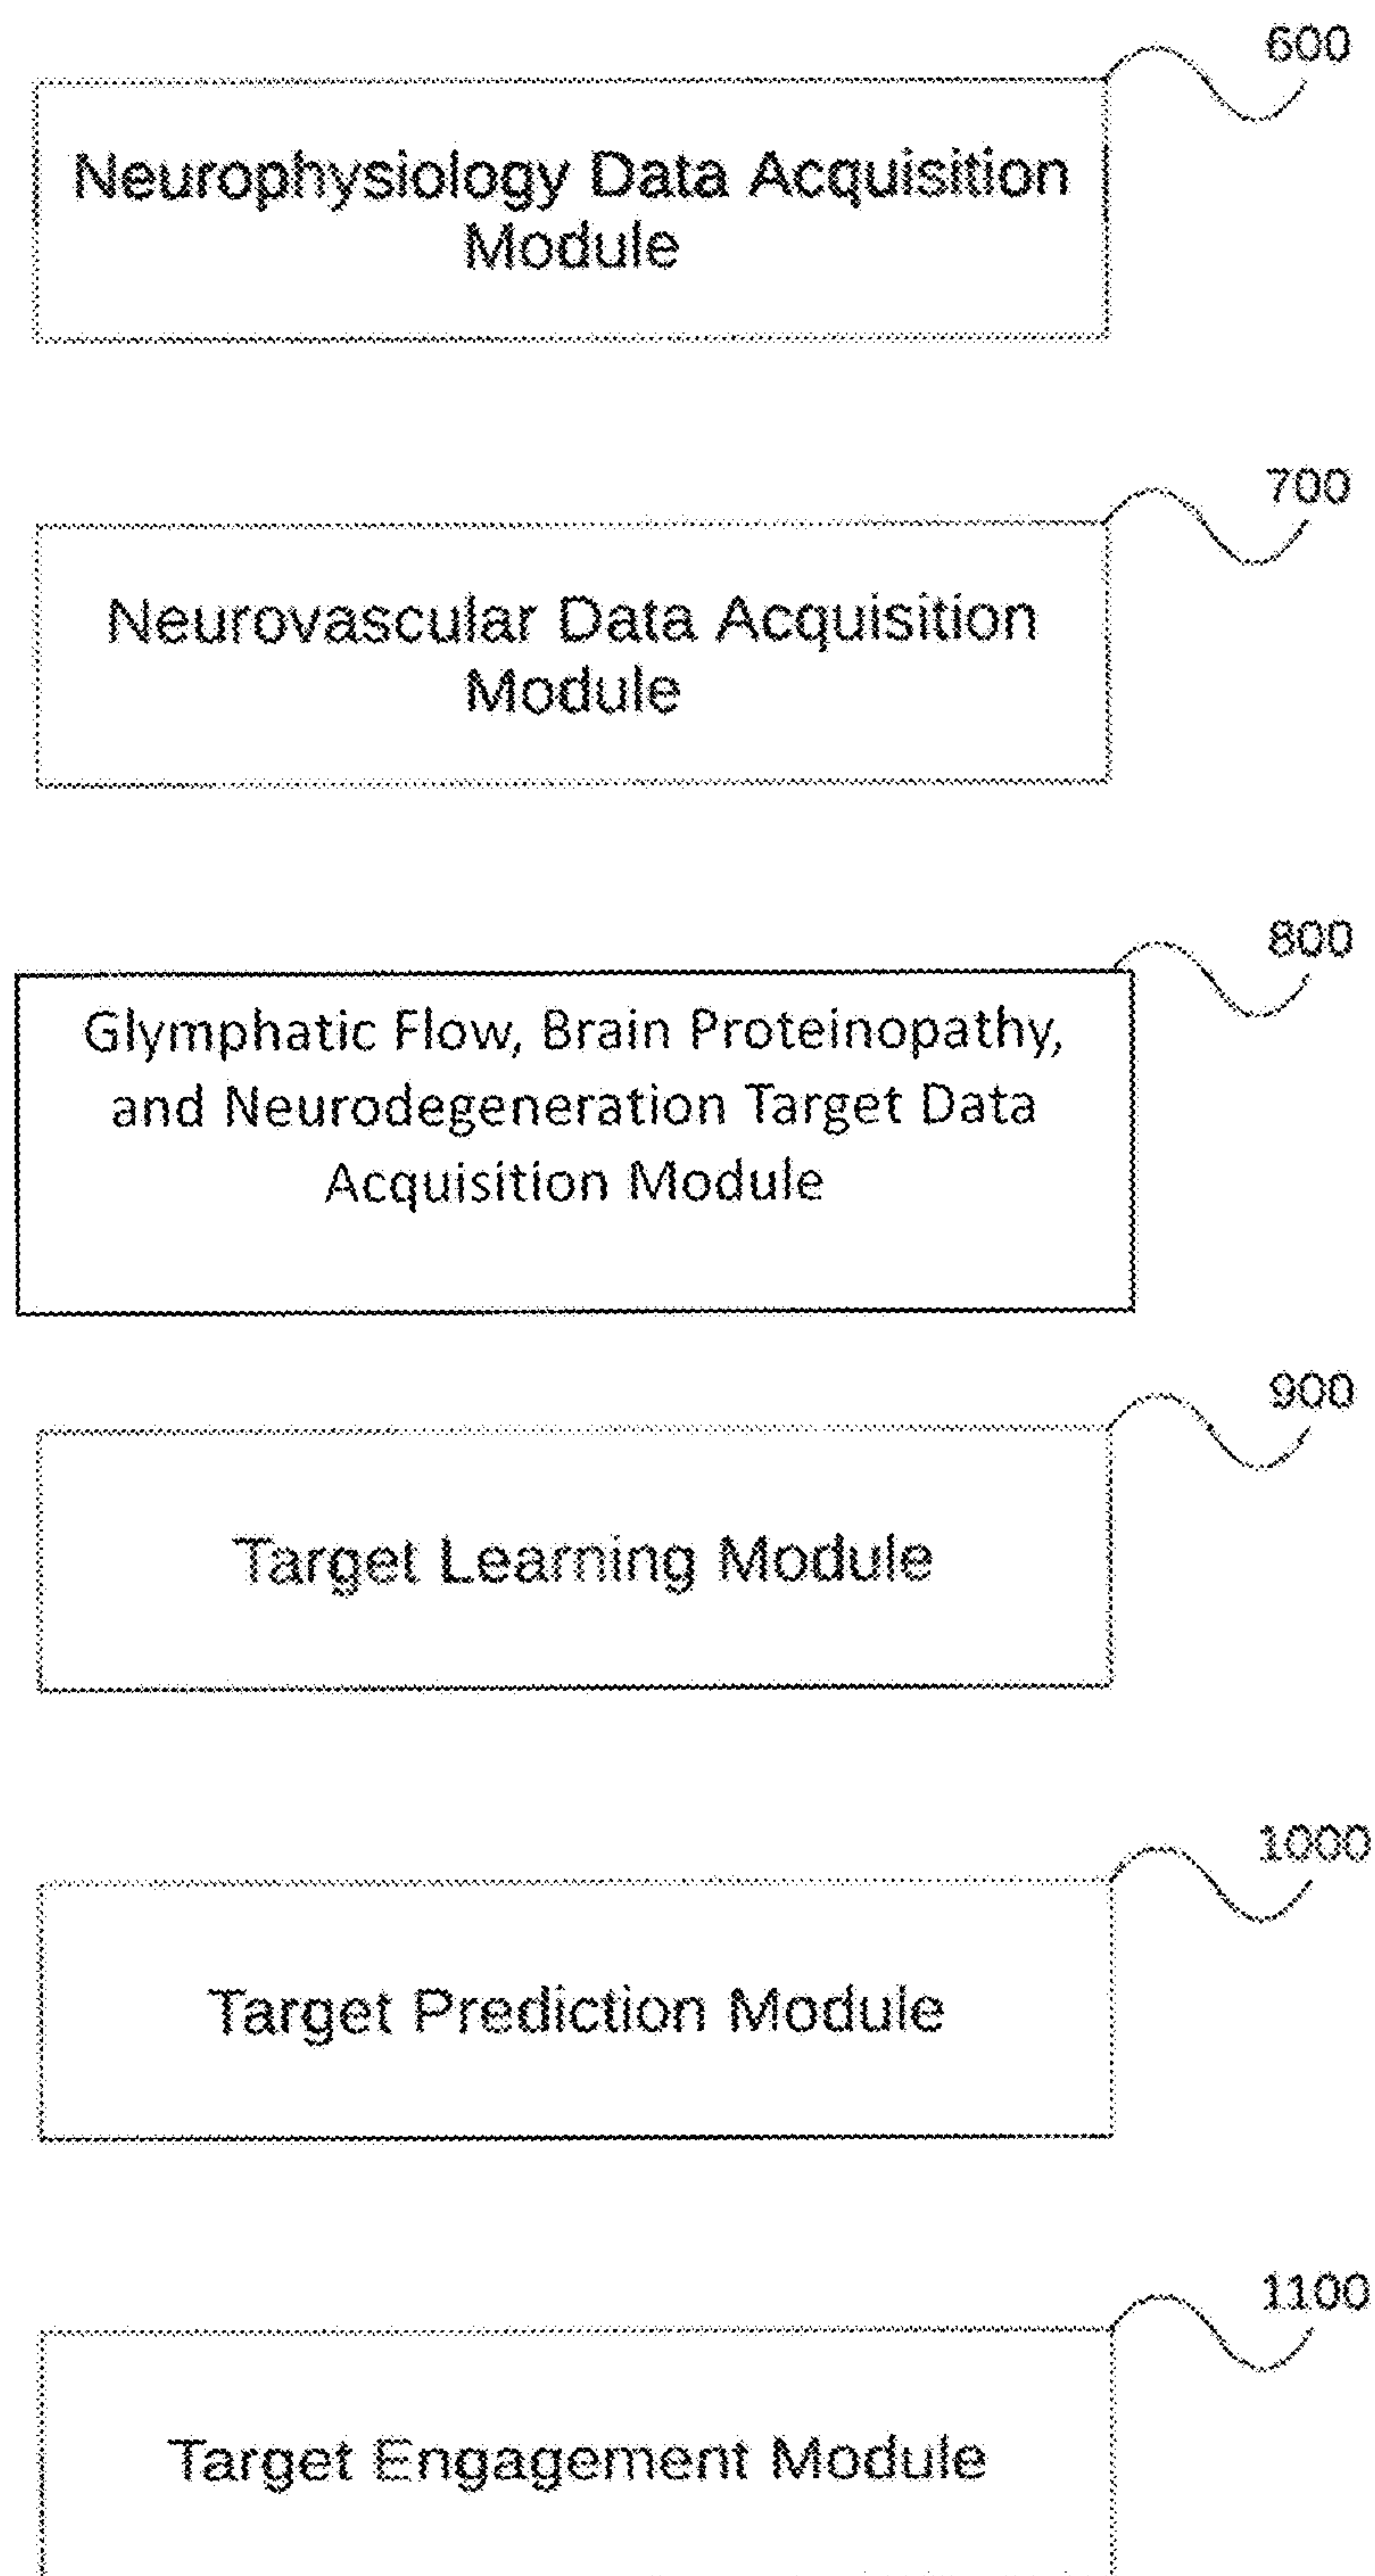


FIG. 4

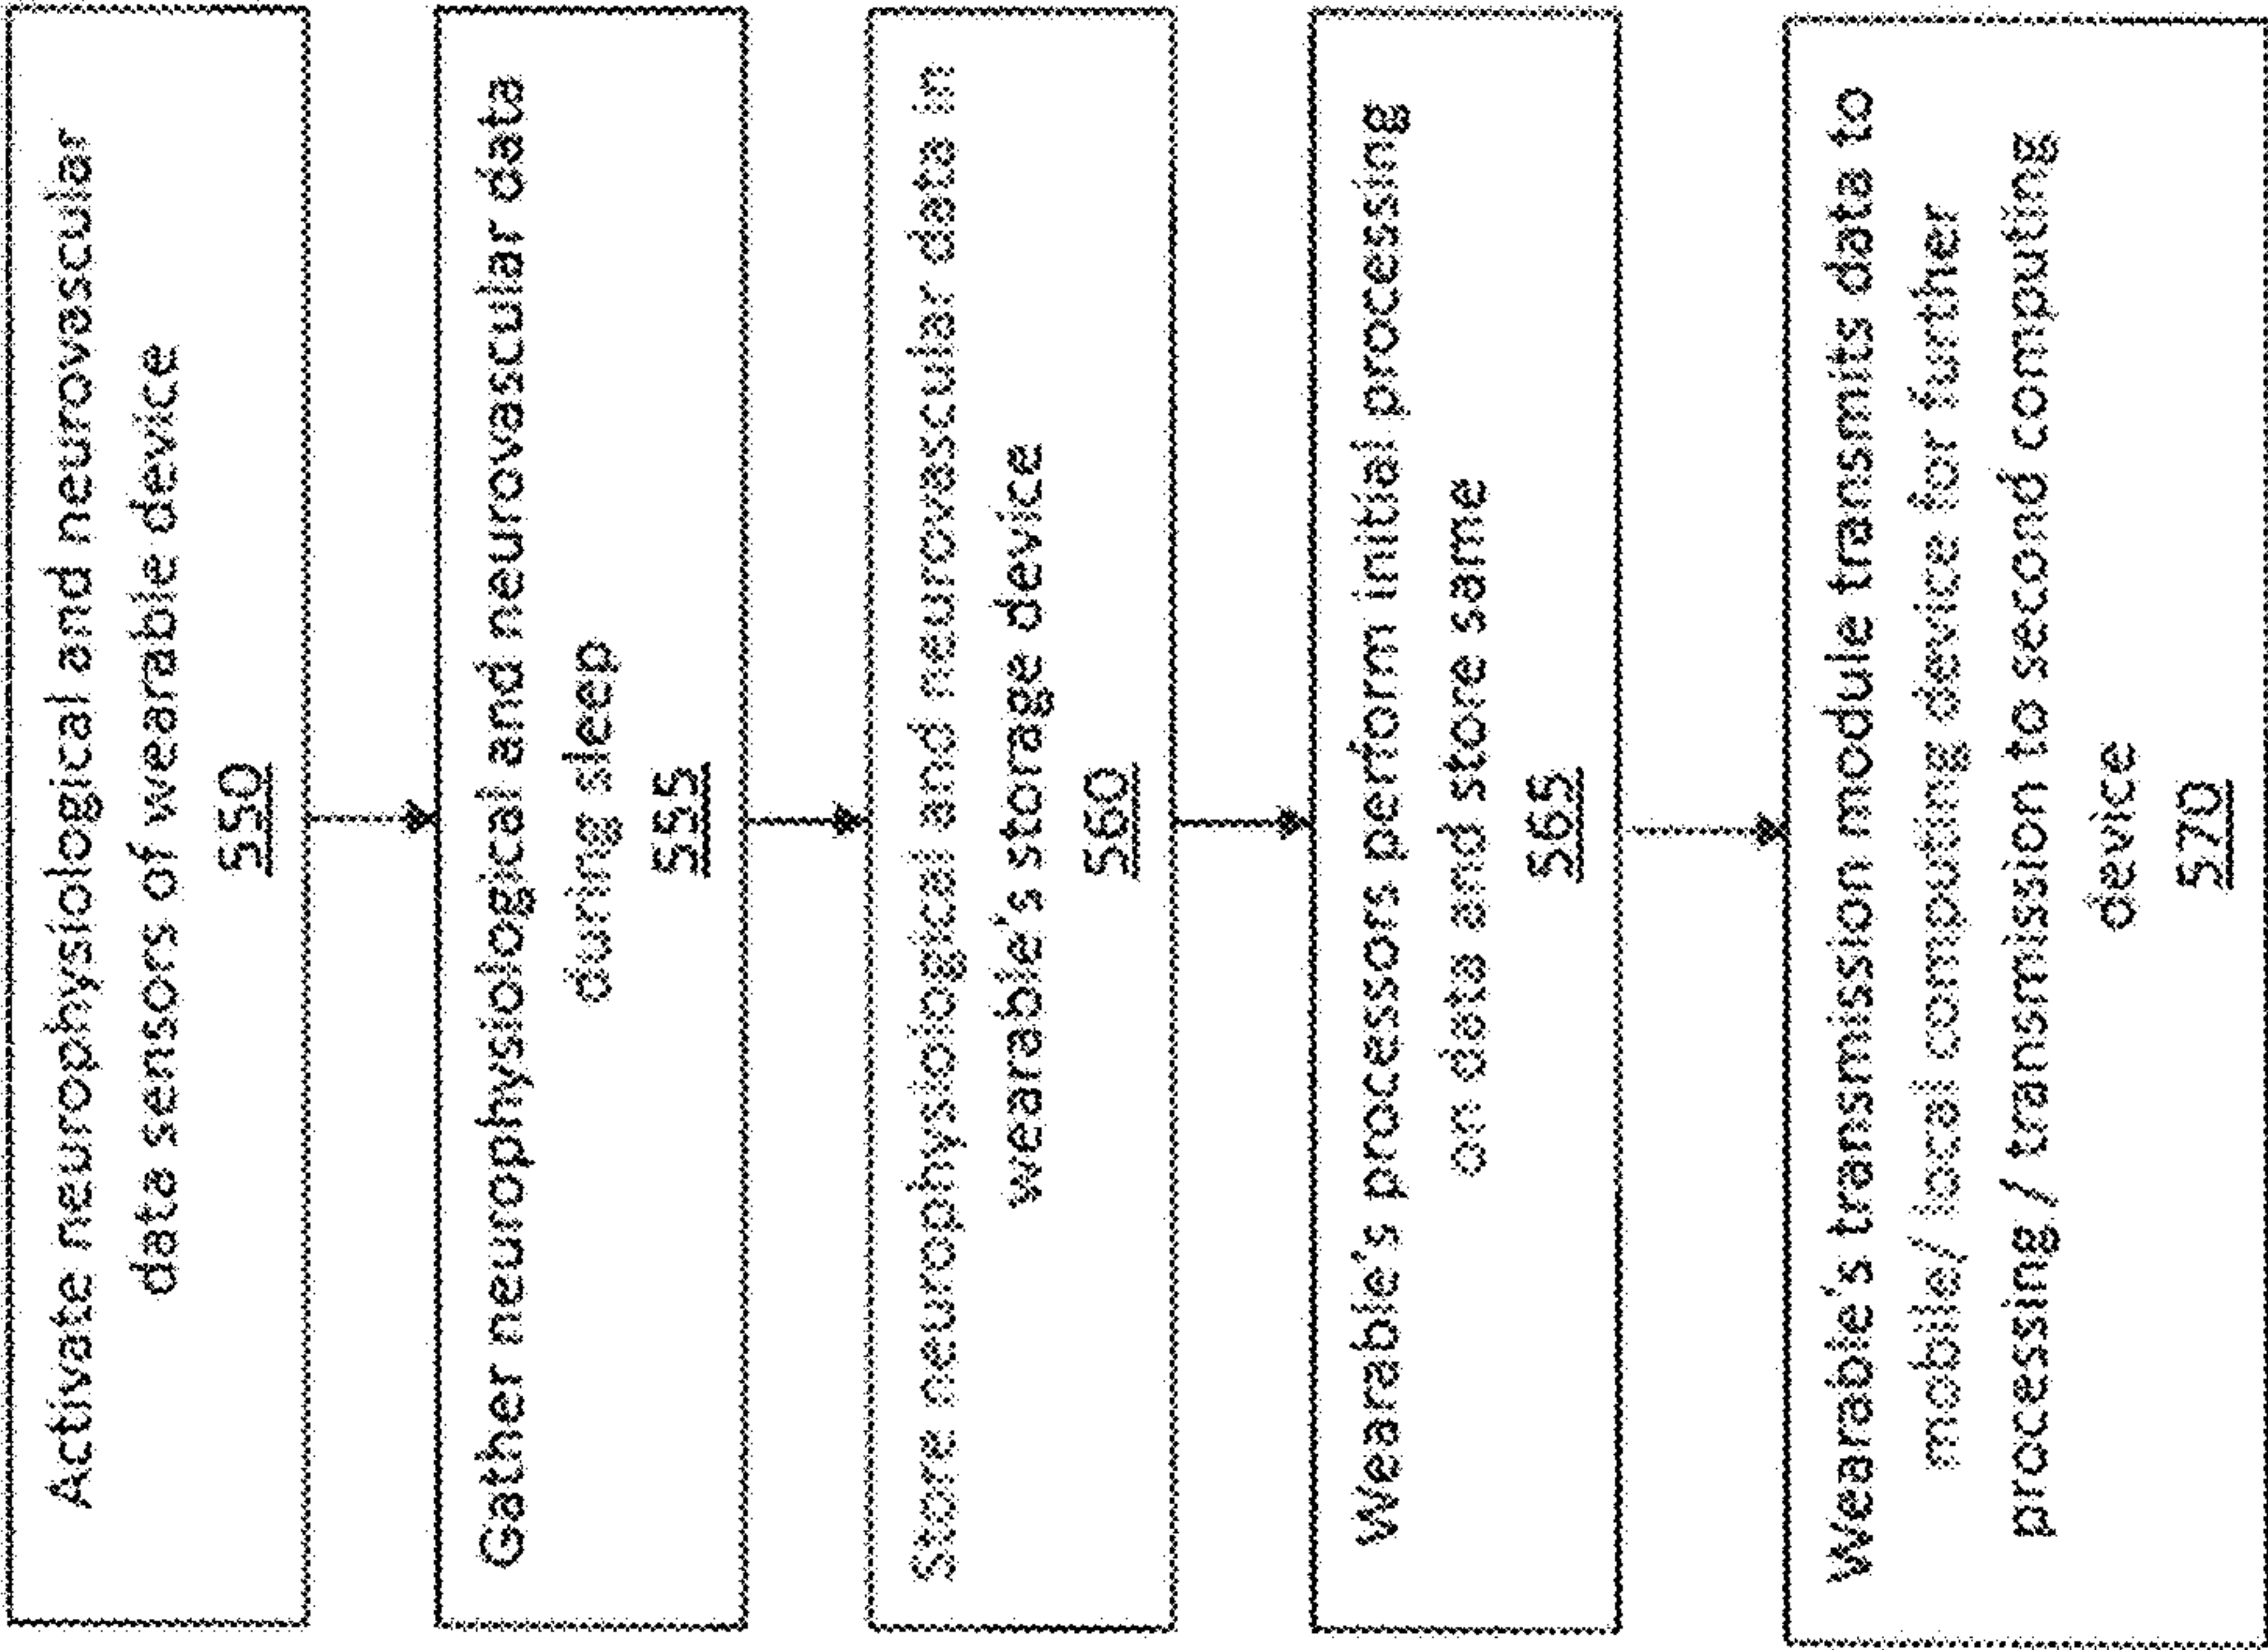


FIG. 5 B

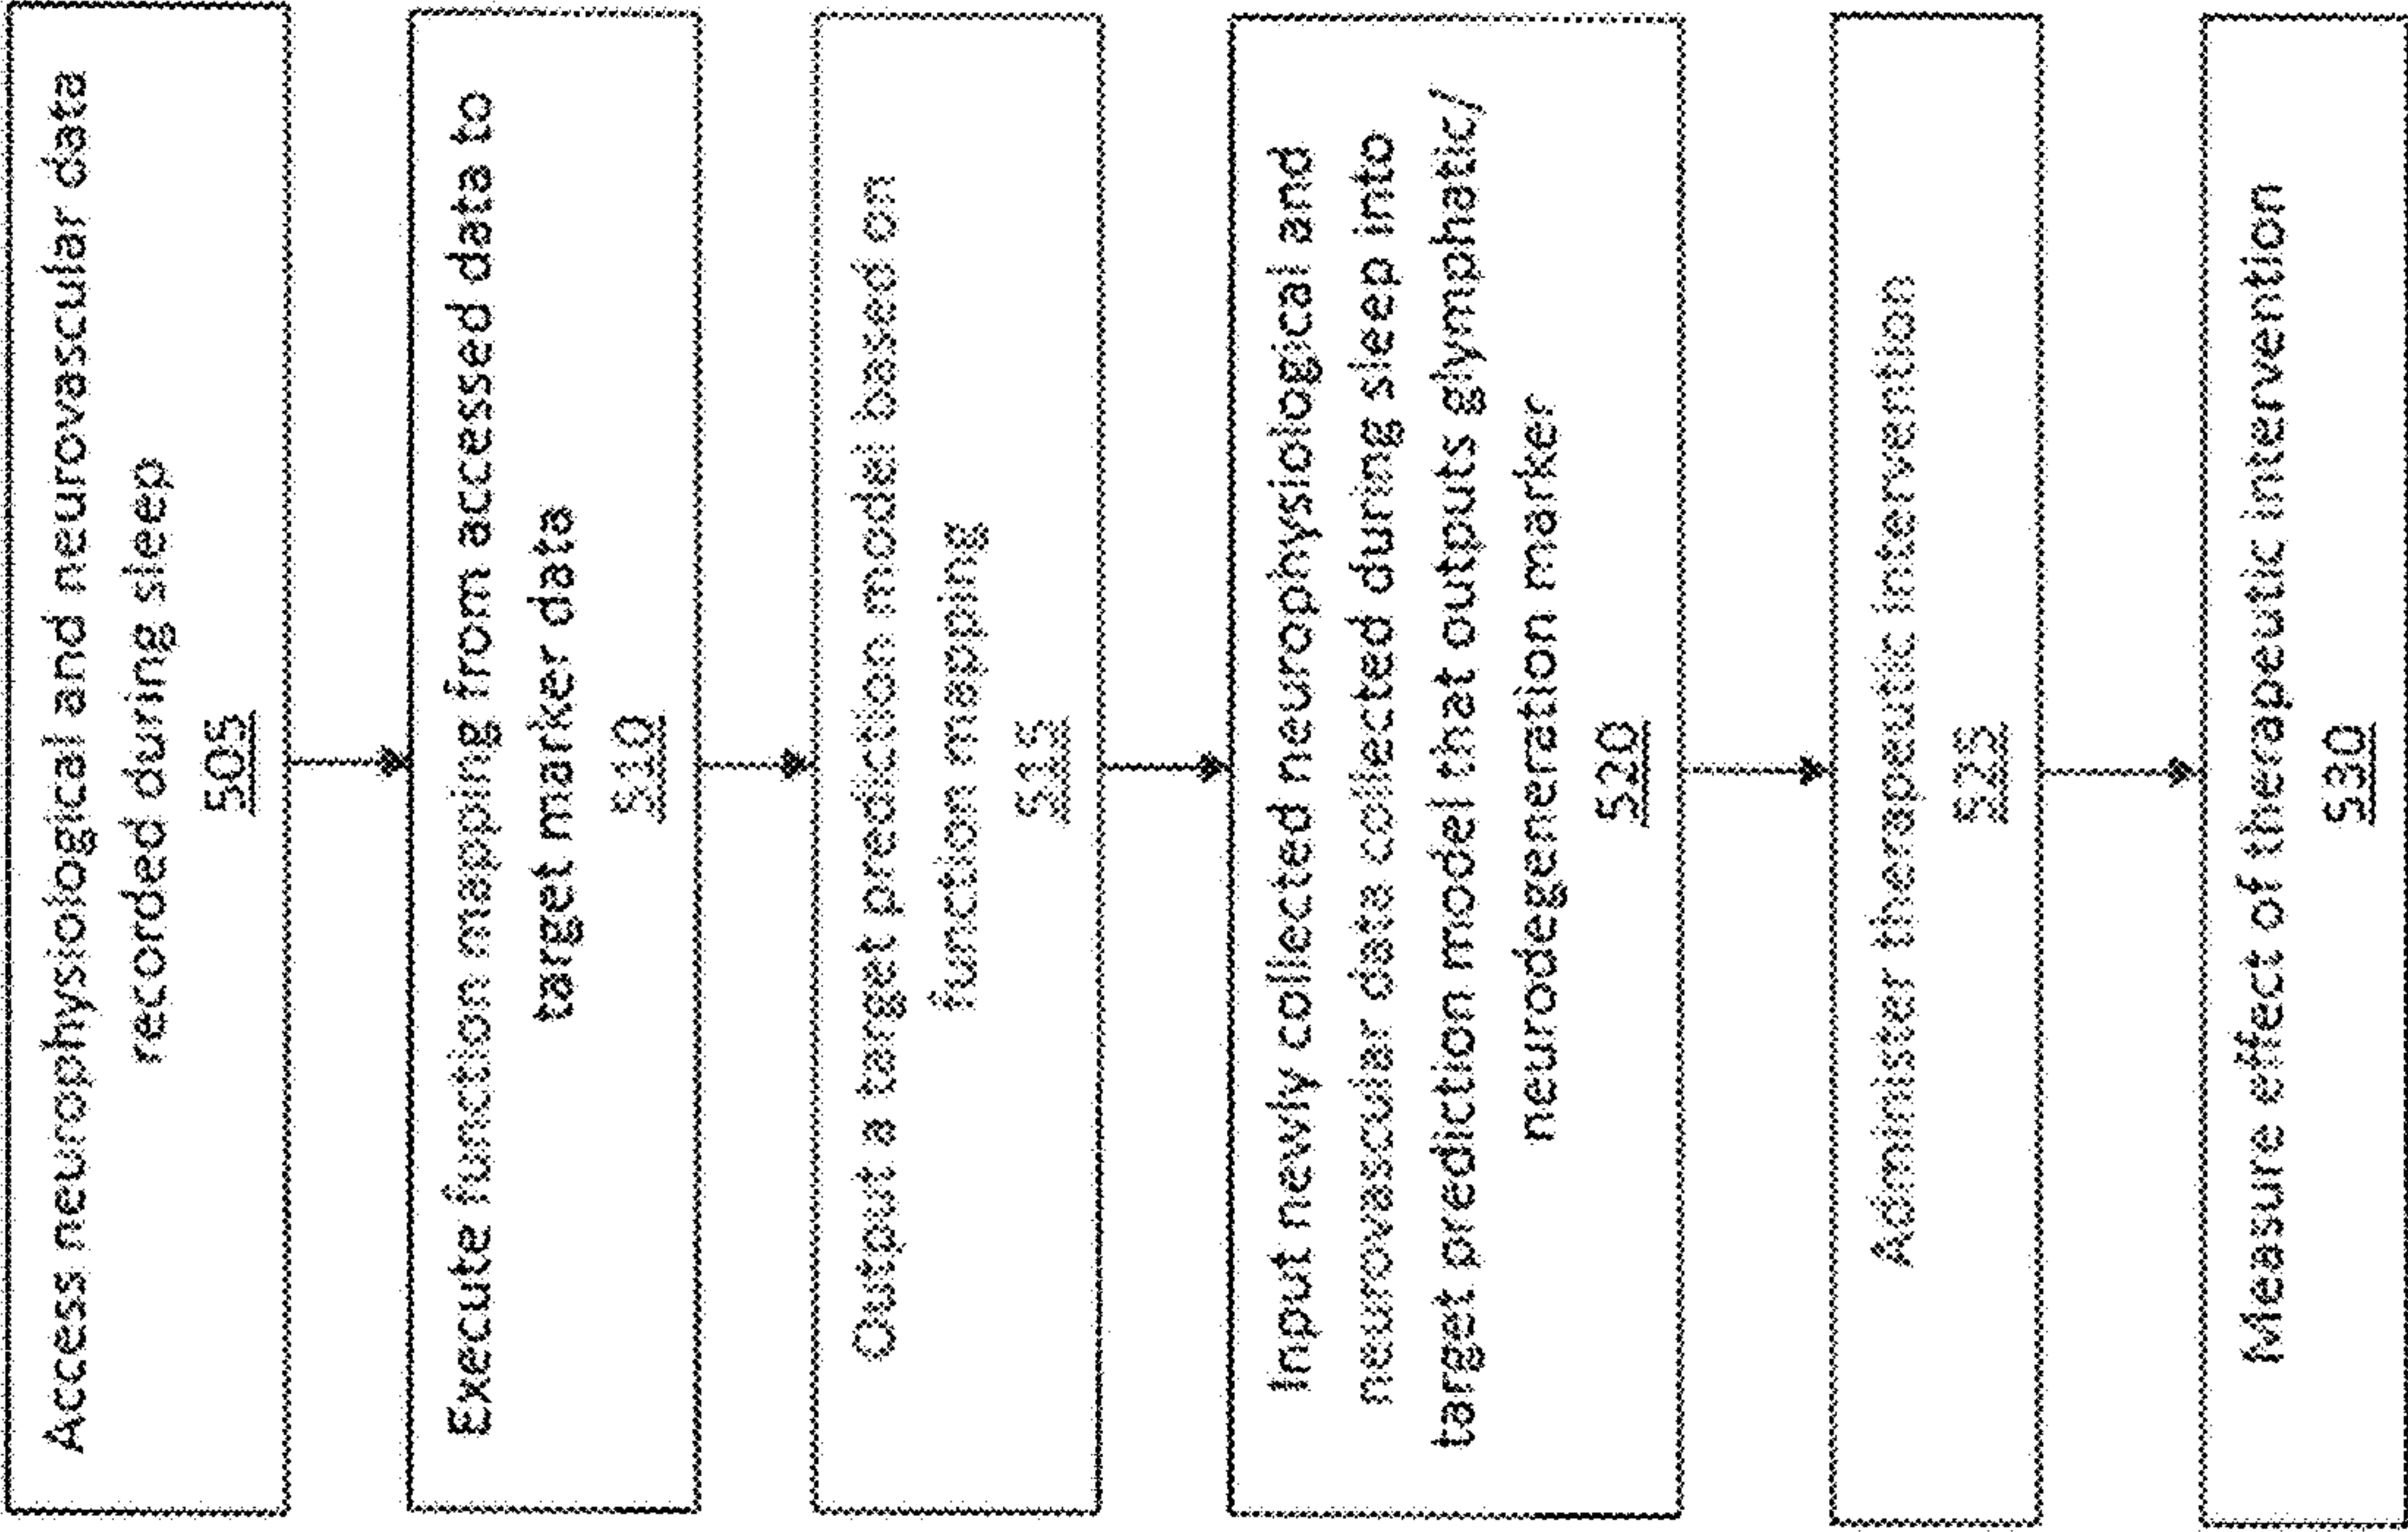


FIG. 5 A

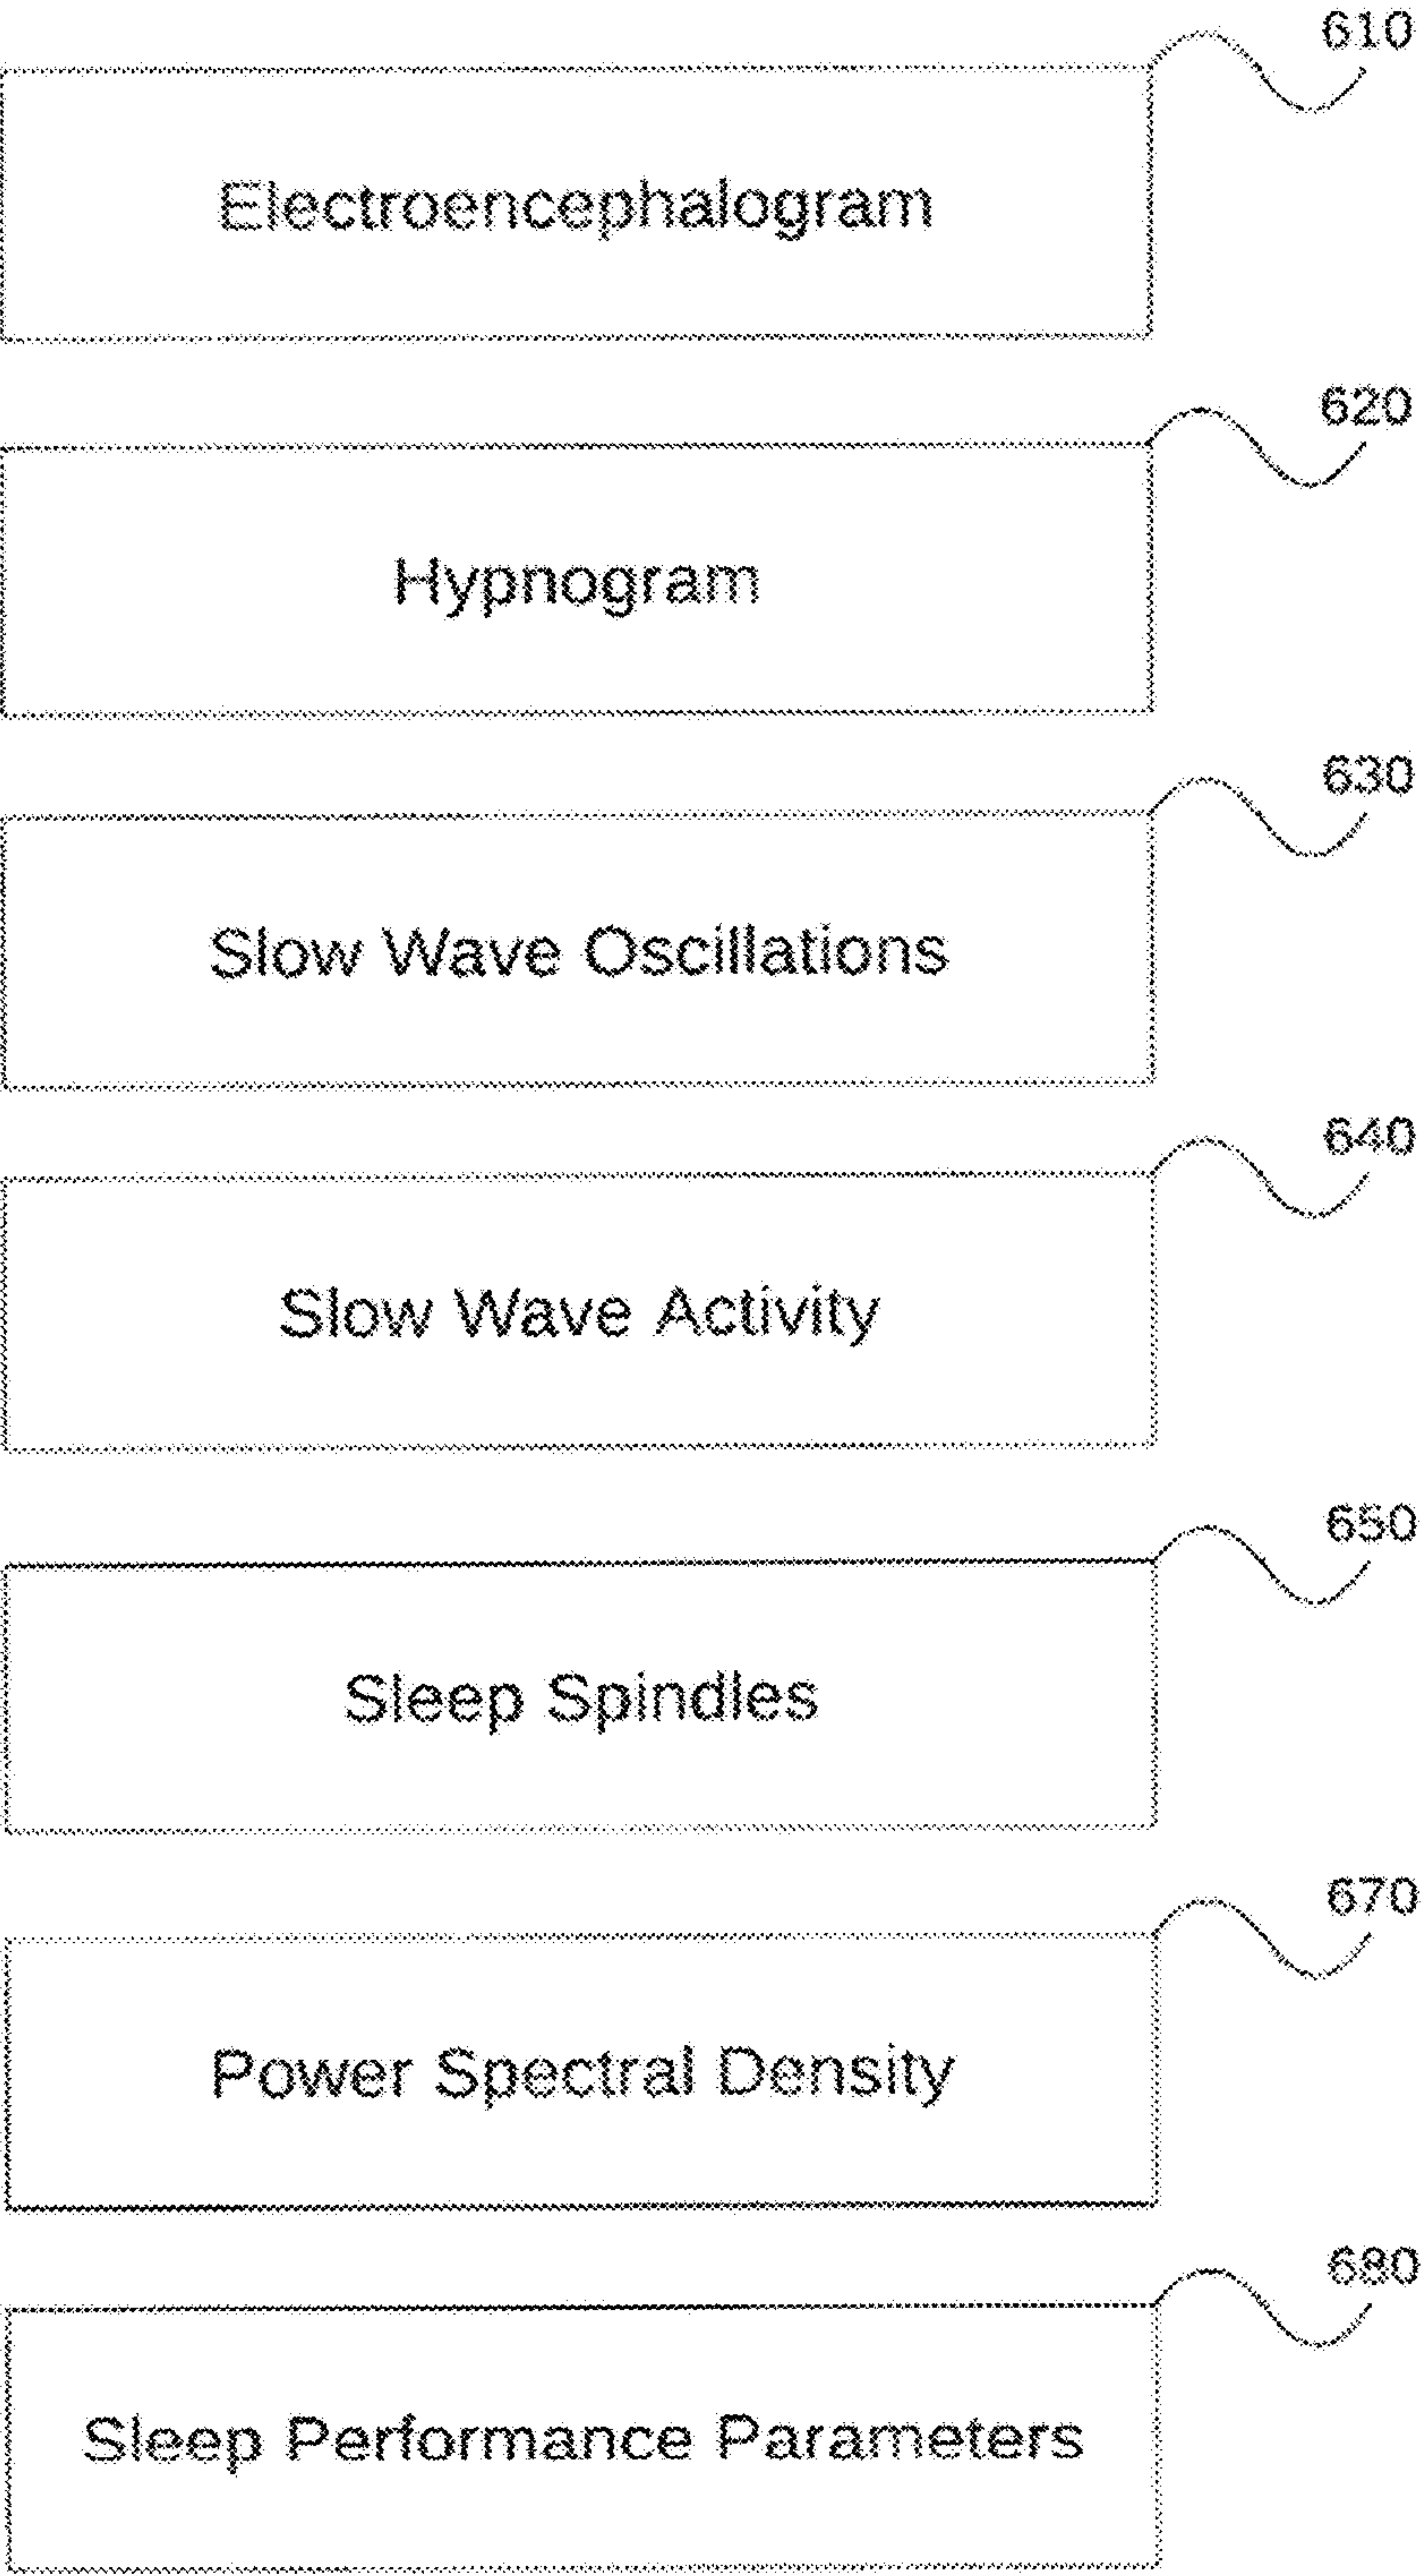
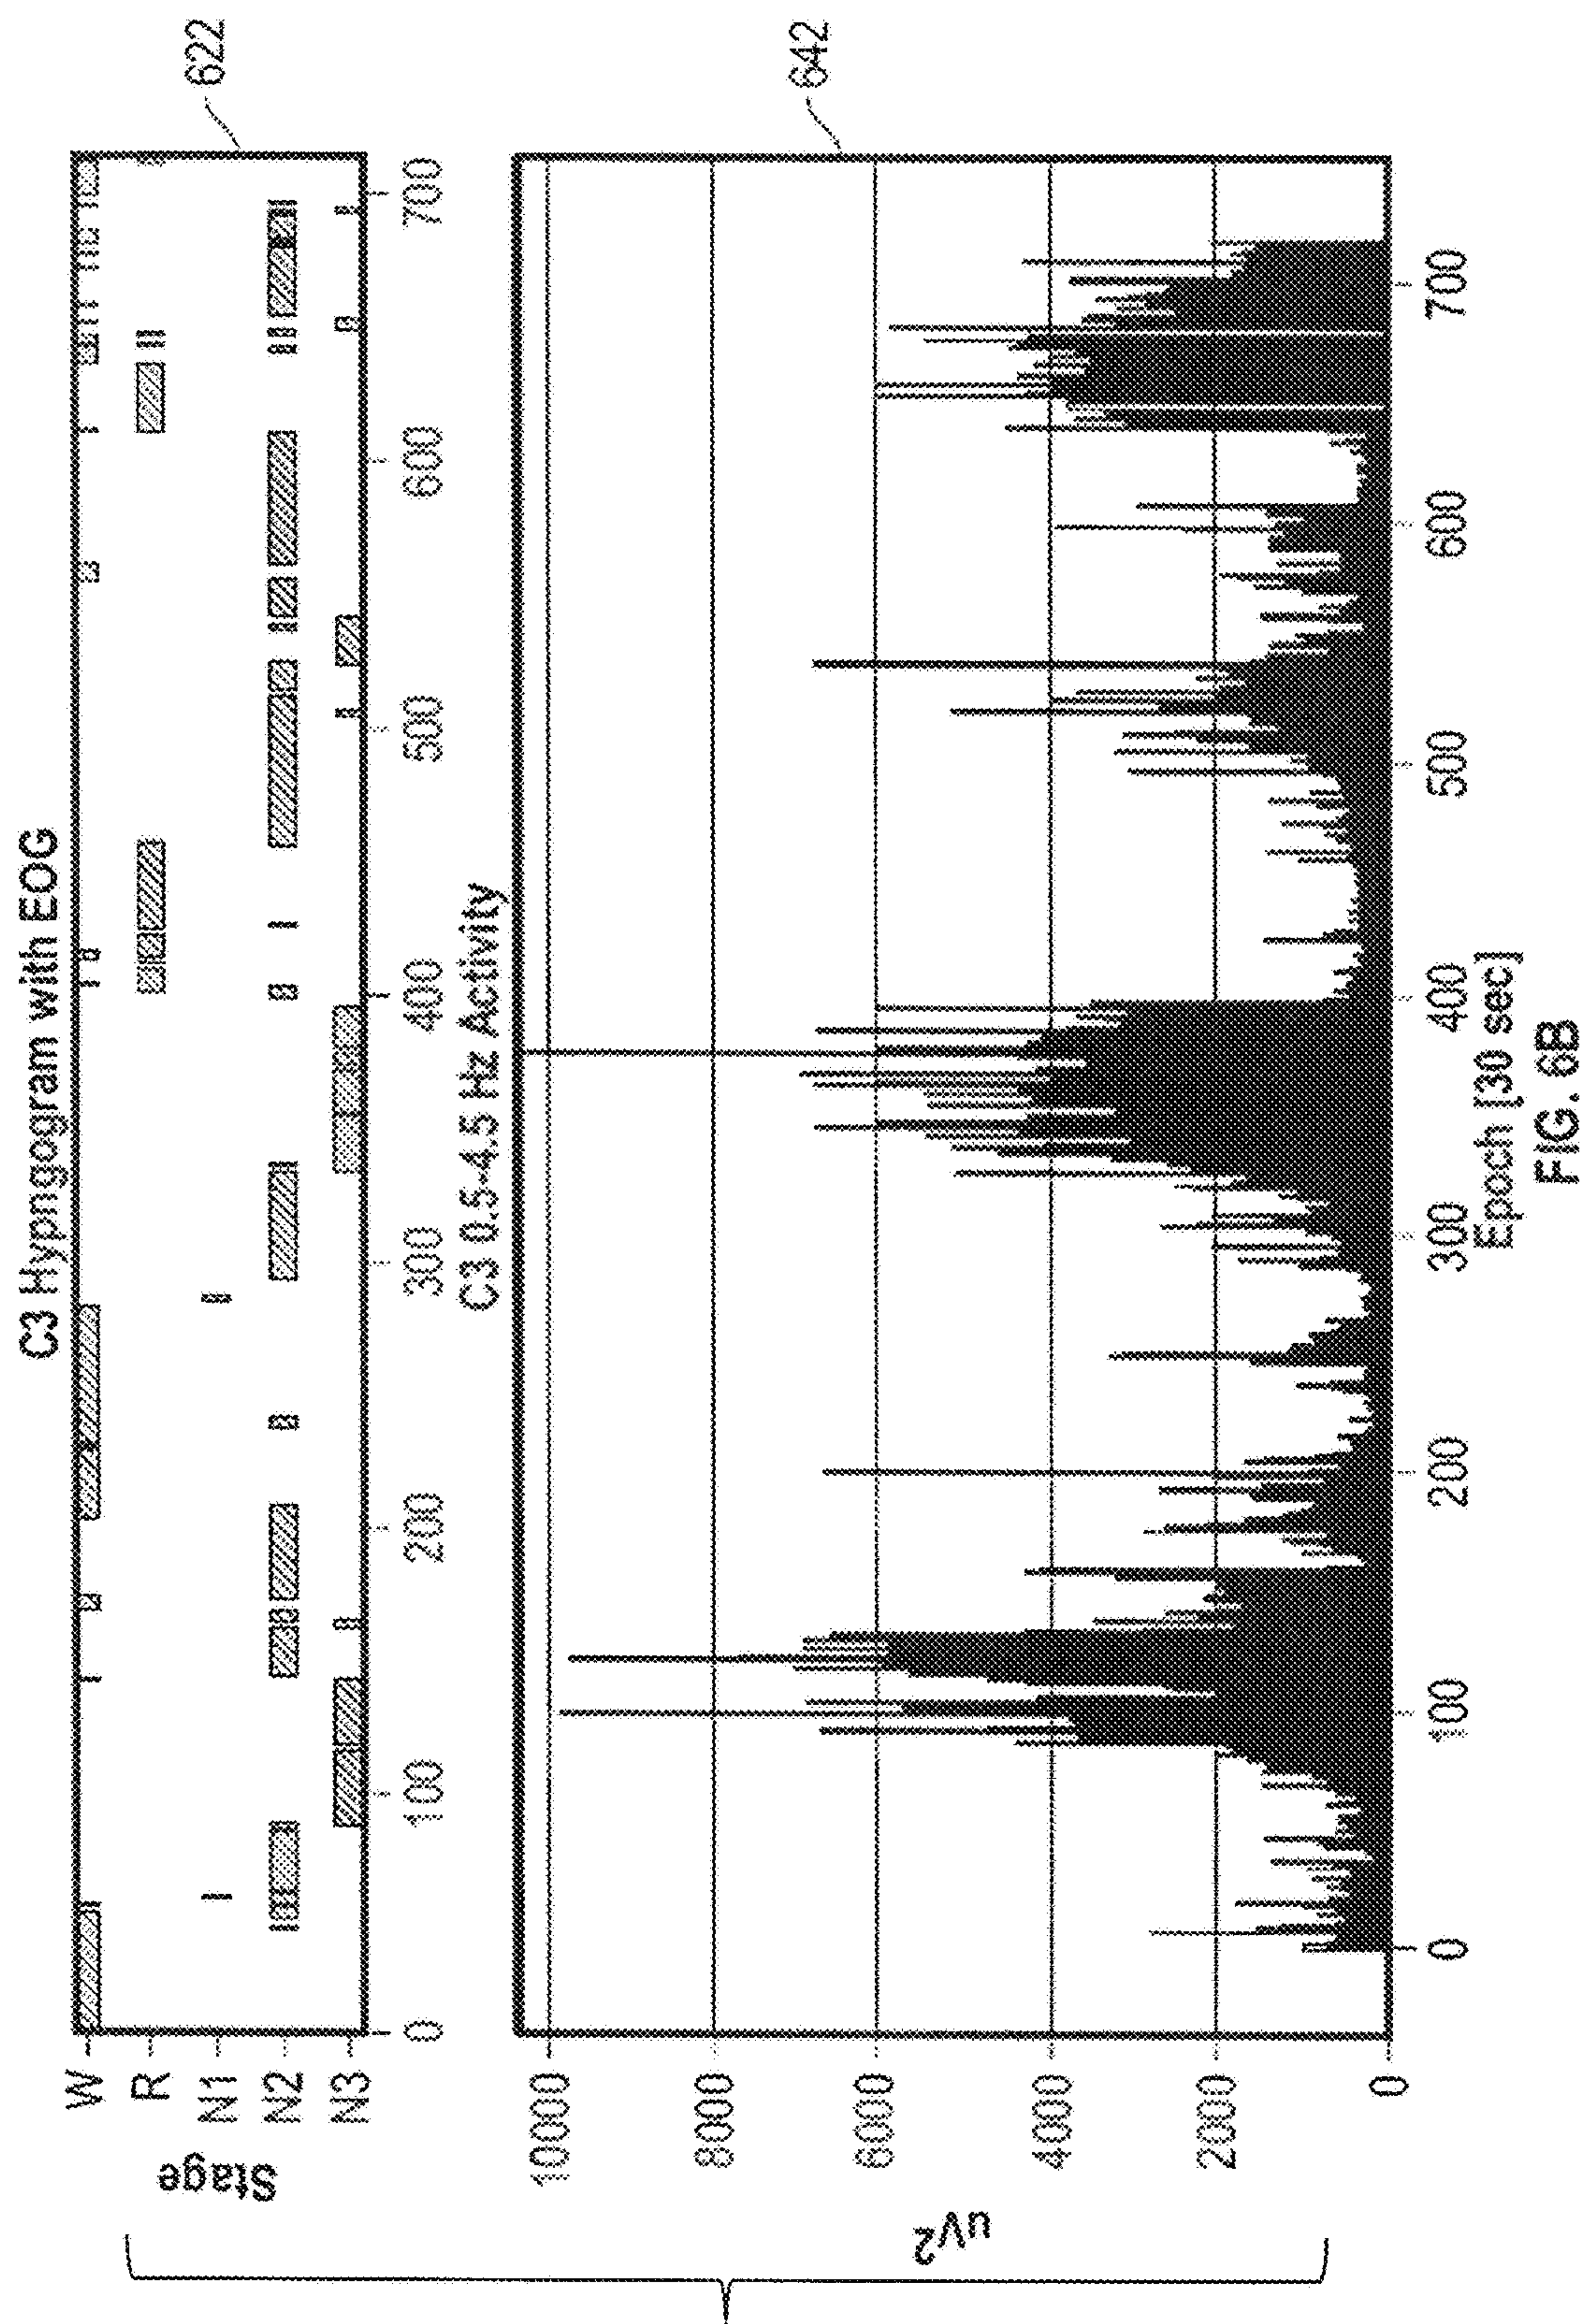


FIG. 6A





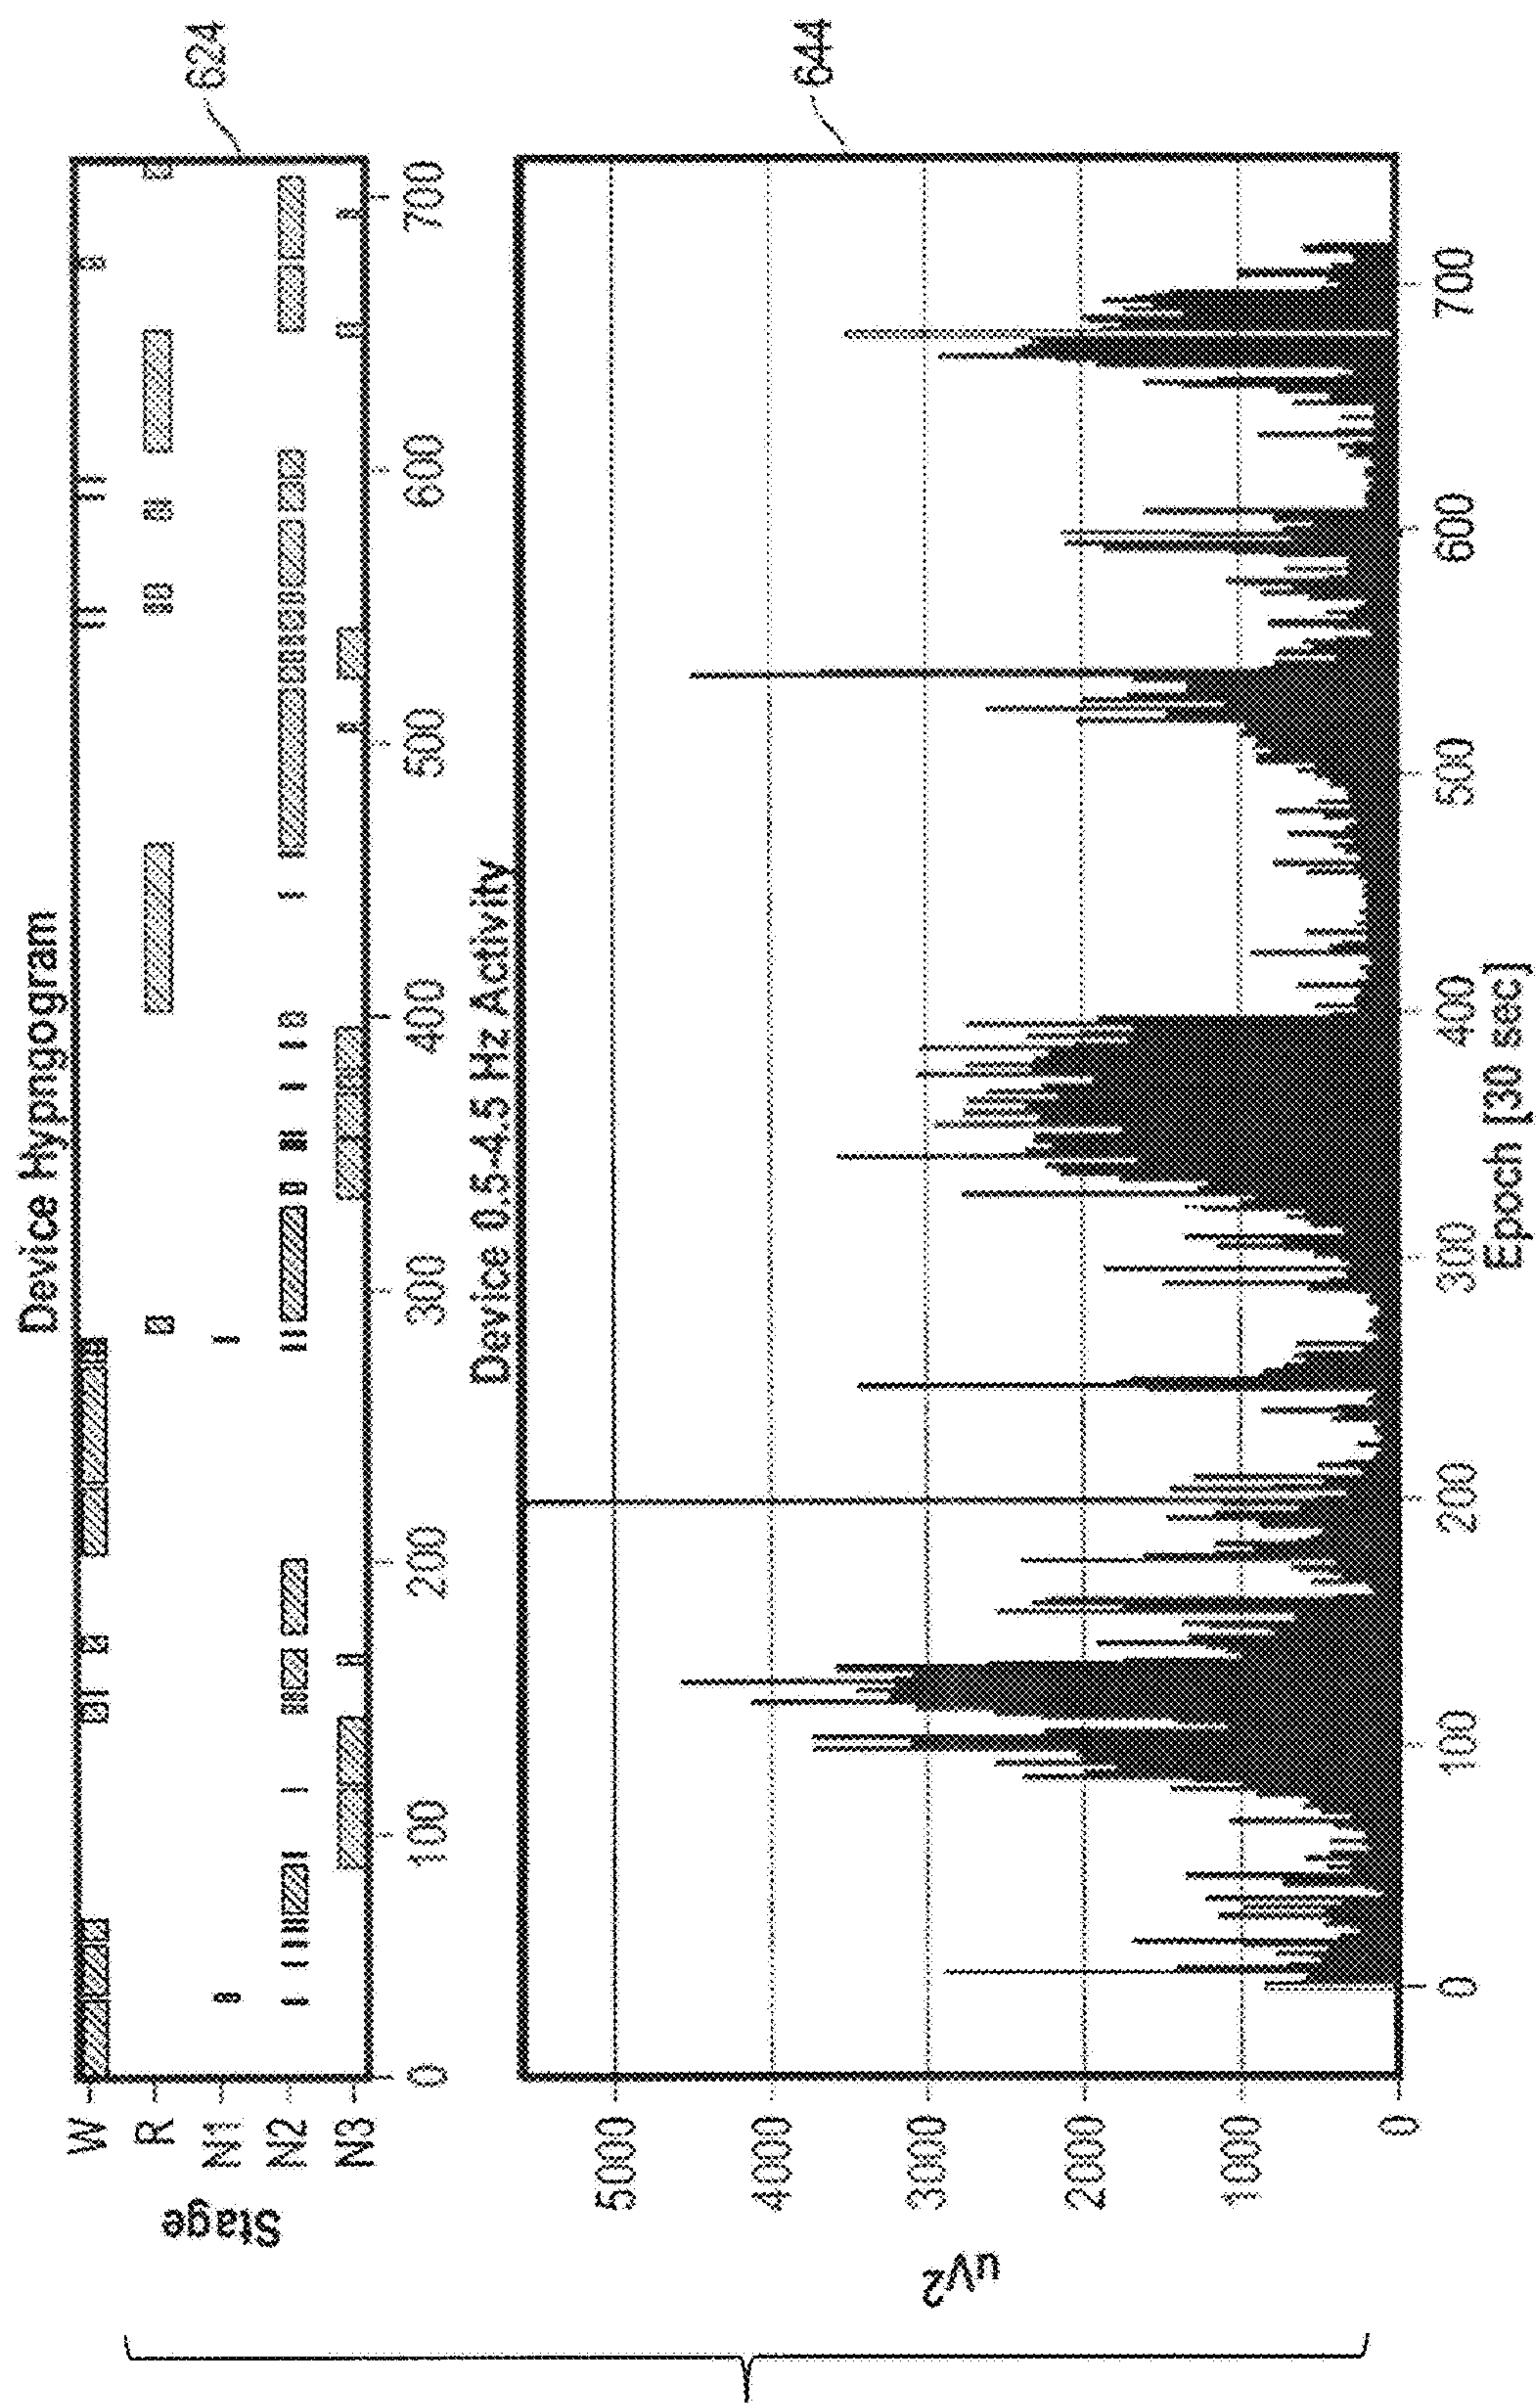


FIG. 6C

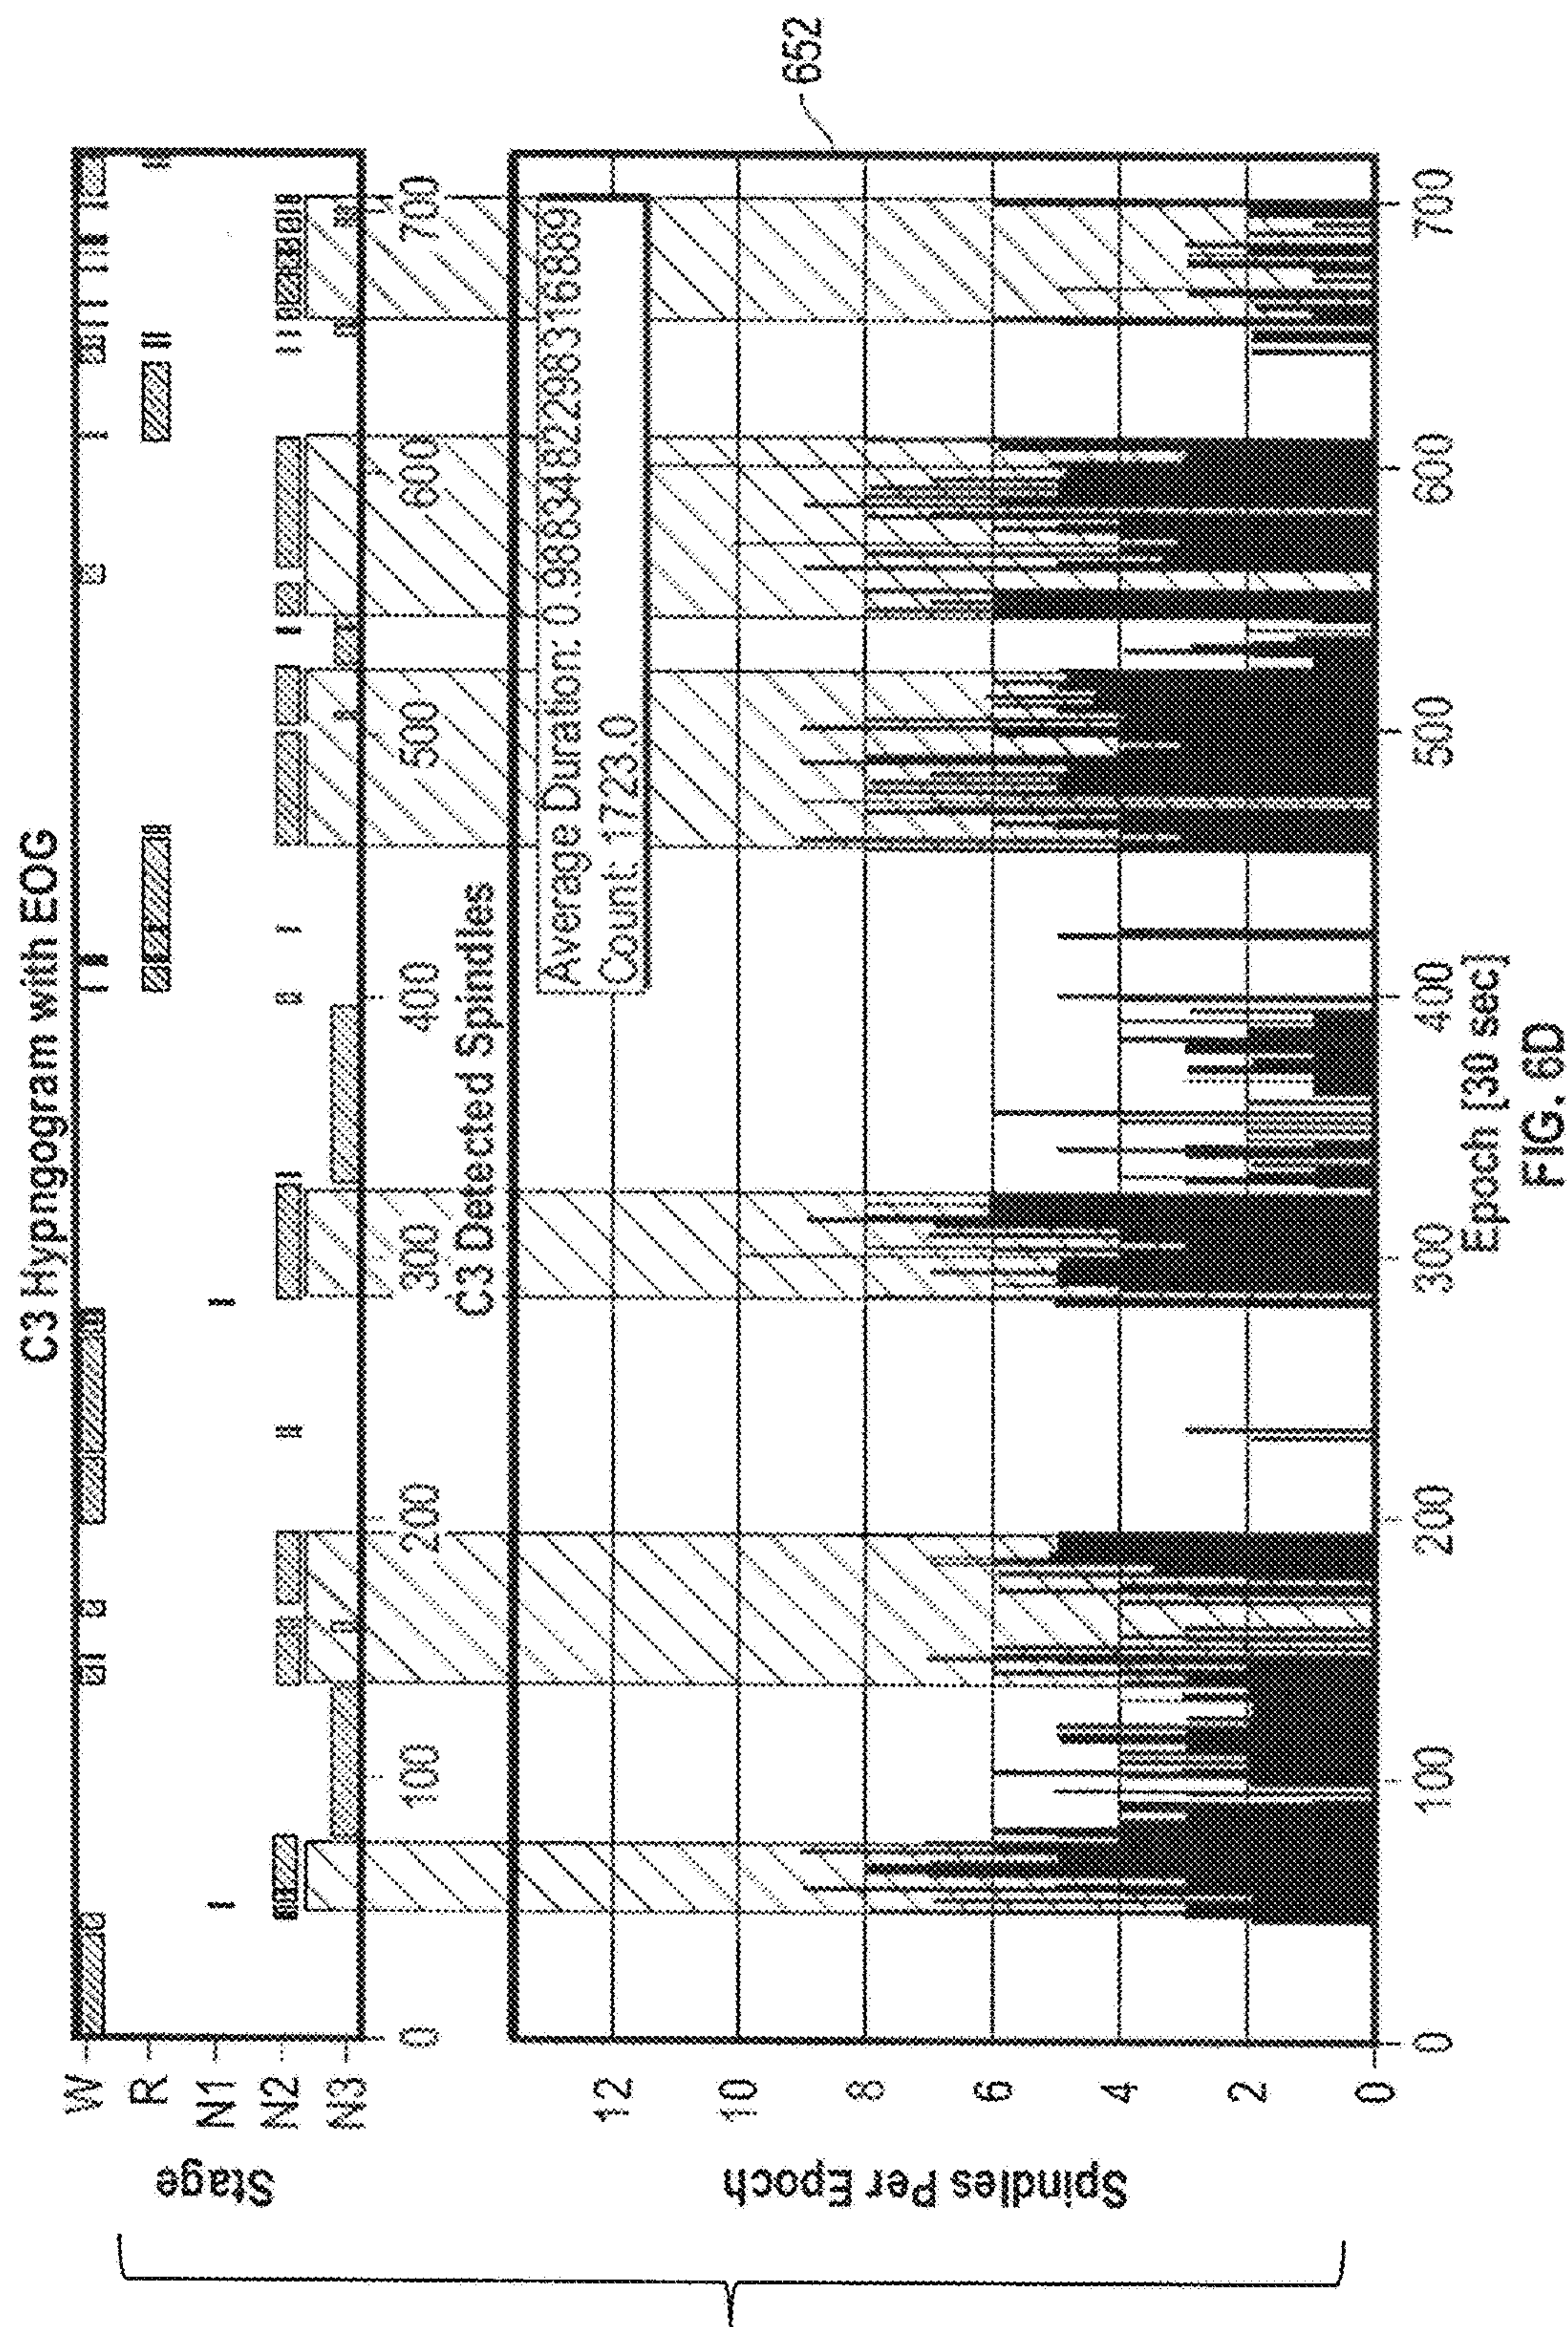

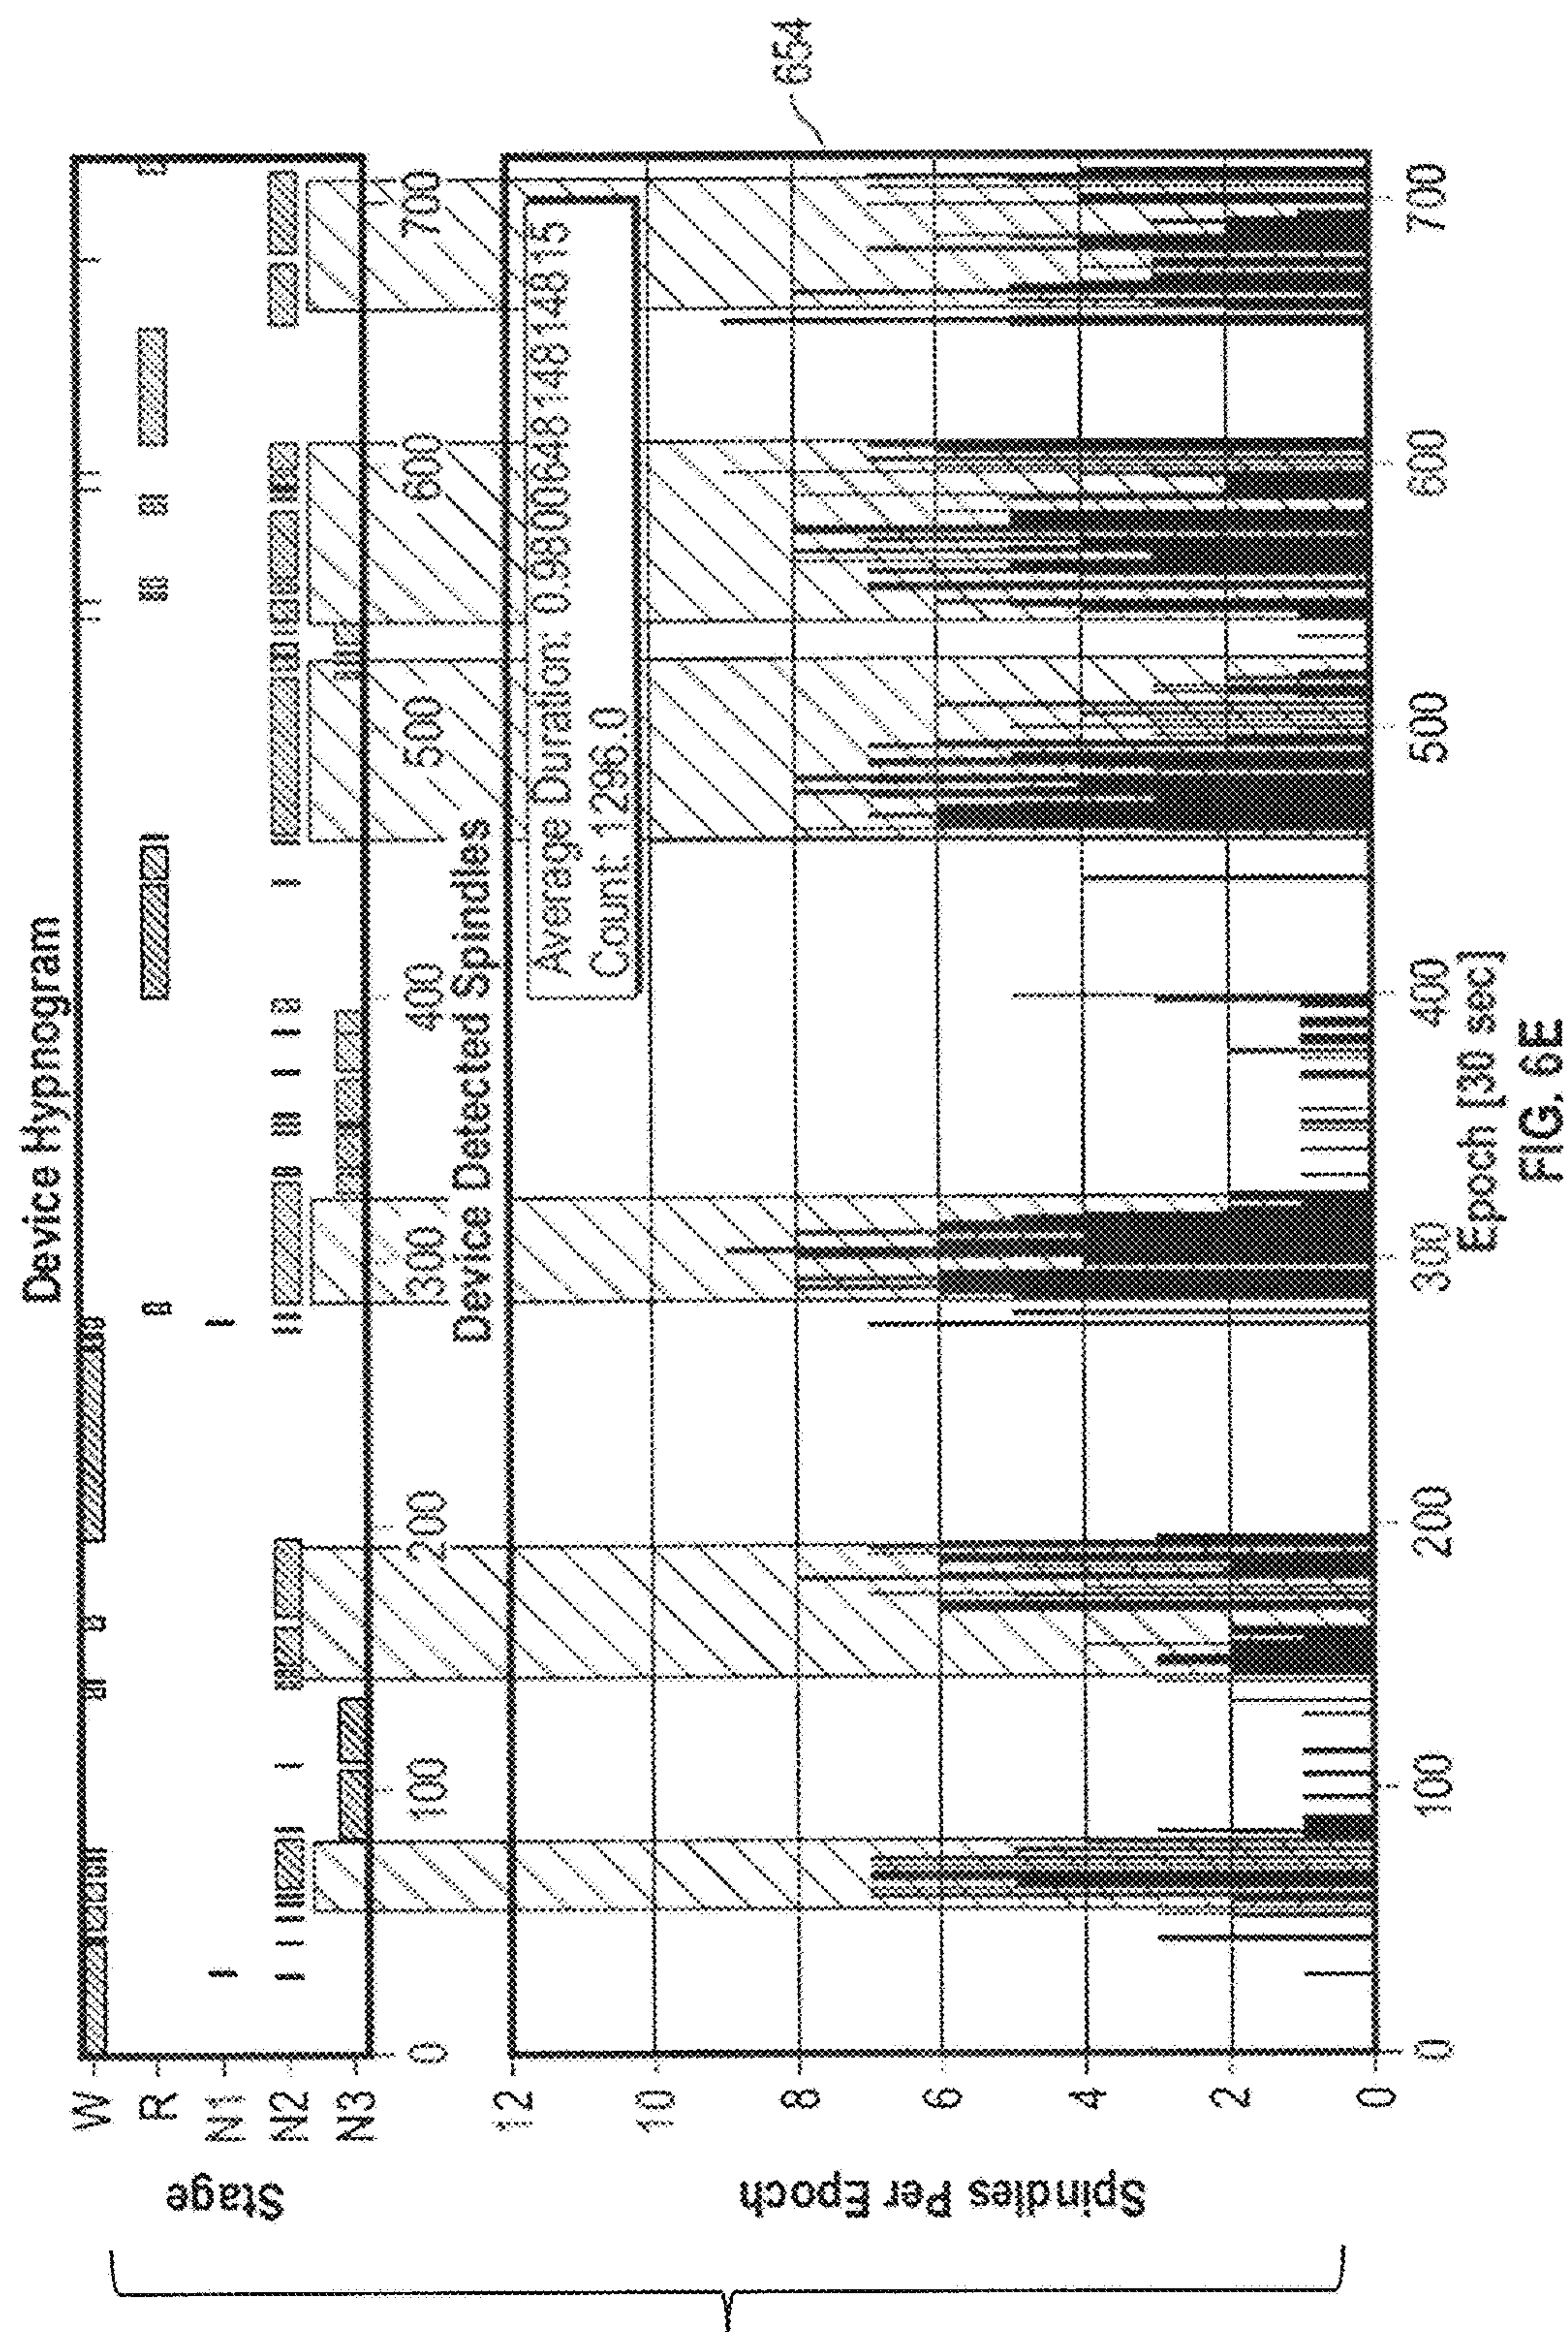

	682													
	<table><tr><th>MEASURE</th><th>Value (%)</th></tr><tr><td>Sensitivity for Wake</td><td>69</td></tr><tr><td>Sensitivity for Light Sleep (N1 or N2)</td><td>80</td></tr><tr><td>Sensitivity for SWS (N3)</td><td>88</td></tr><tr><td>Sensitivity for REM</td><td>99</td></tr><tr><td>Overall agreement</td><td>81</td></tr></table>		MEASURE	Value (%)	Sensitivity for Wake	69	Sensitivity for Light Sleep (N1 or N2)	80	Sensitivity for SWS (N3)	88	Sensitivity for REM	99	Overall agreement	81
	MEASURE	Value (%)												
	Sensitivity for Wake	69												
	Sensitivity for Light Sleep (N1 or N2)	80												
	Sensitivity for SWS (N3)	88												
	Sensitivity for REM	99												
Overall agreement	81													

	684																				
	<table><tr><th>MEASURE</th><th>EEG</th><th>Device</th></tr><tr><td>Total Sleep Time (min)</td><td>270</td><td>282</td></tr><tr><td>Sleep Onset Latency (min)</td><td>23</td><td>23</td></tr><tr><td>Wake After Sleep Onset (min)</td><td>65</td><td>62</td></tr><tr><td>Sleep Efficiency (%)</td><td>75</td><td>79</td></tr><tr><td>Number of Awakenings</td><td>22</td><td>18</td></tr></table>			MEASURE	EEG	Device	Total Sleep Time (min)	270	282	Sleep Onset Latency (min)	23	23	Wake After Sleep Onset (min)	65	62	Sleep Efficiency (%)	75	79	Number of Awakenings	22	18
	MEASURE	EEG	Device																		
	Total Sleep Time (min)	270	282																		
	Sleep Onset Latency (min)	23	23																		
	Wake After Sleep Onset (min)	65	62																		
	Sleep Efficiency (%)	75	79																		
Number of Awakenings	22	18																			

FIG. 6F

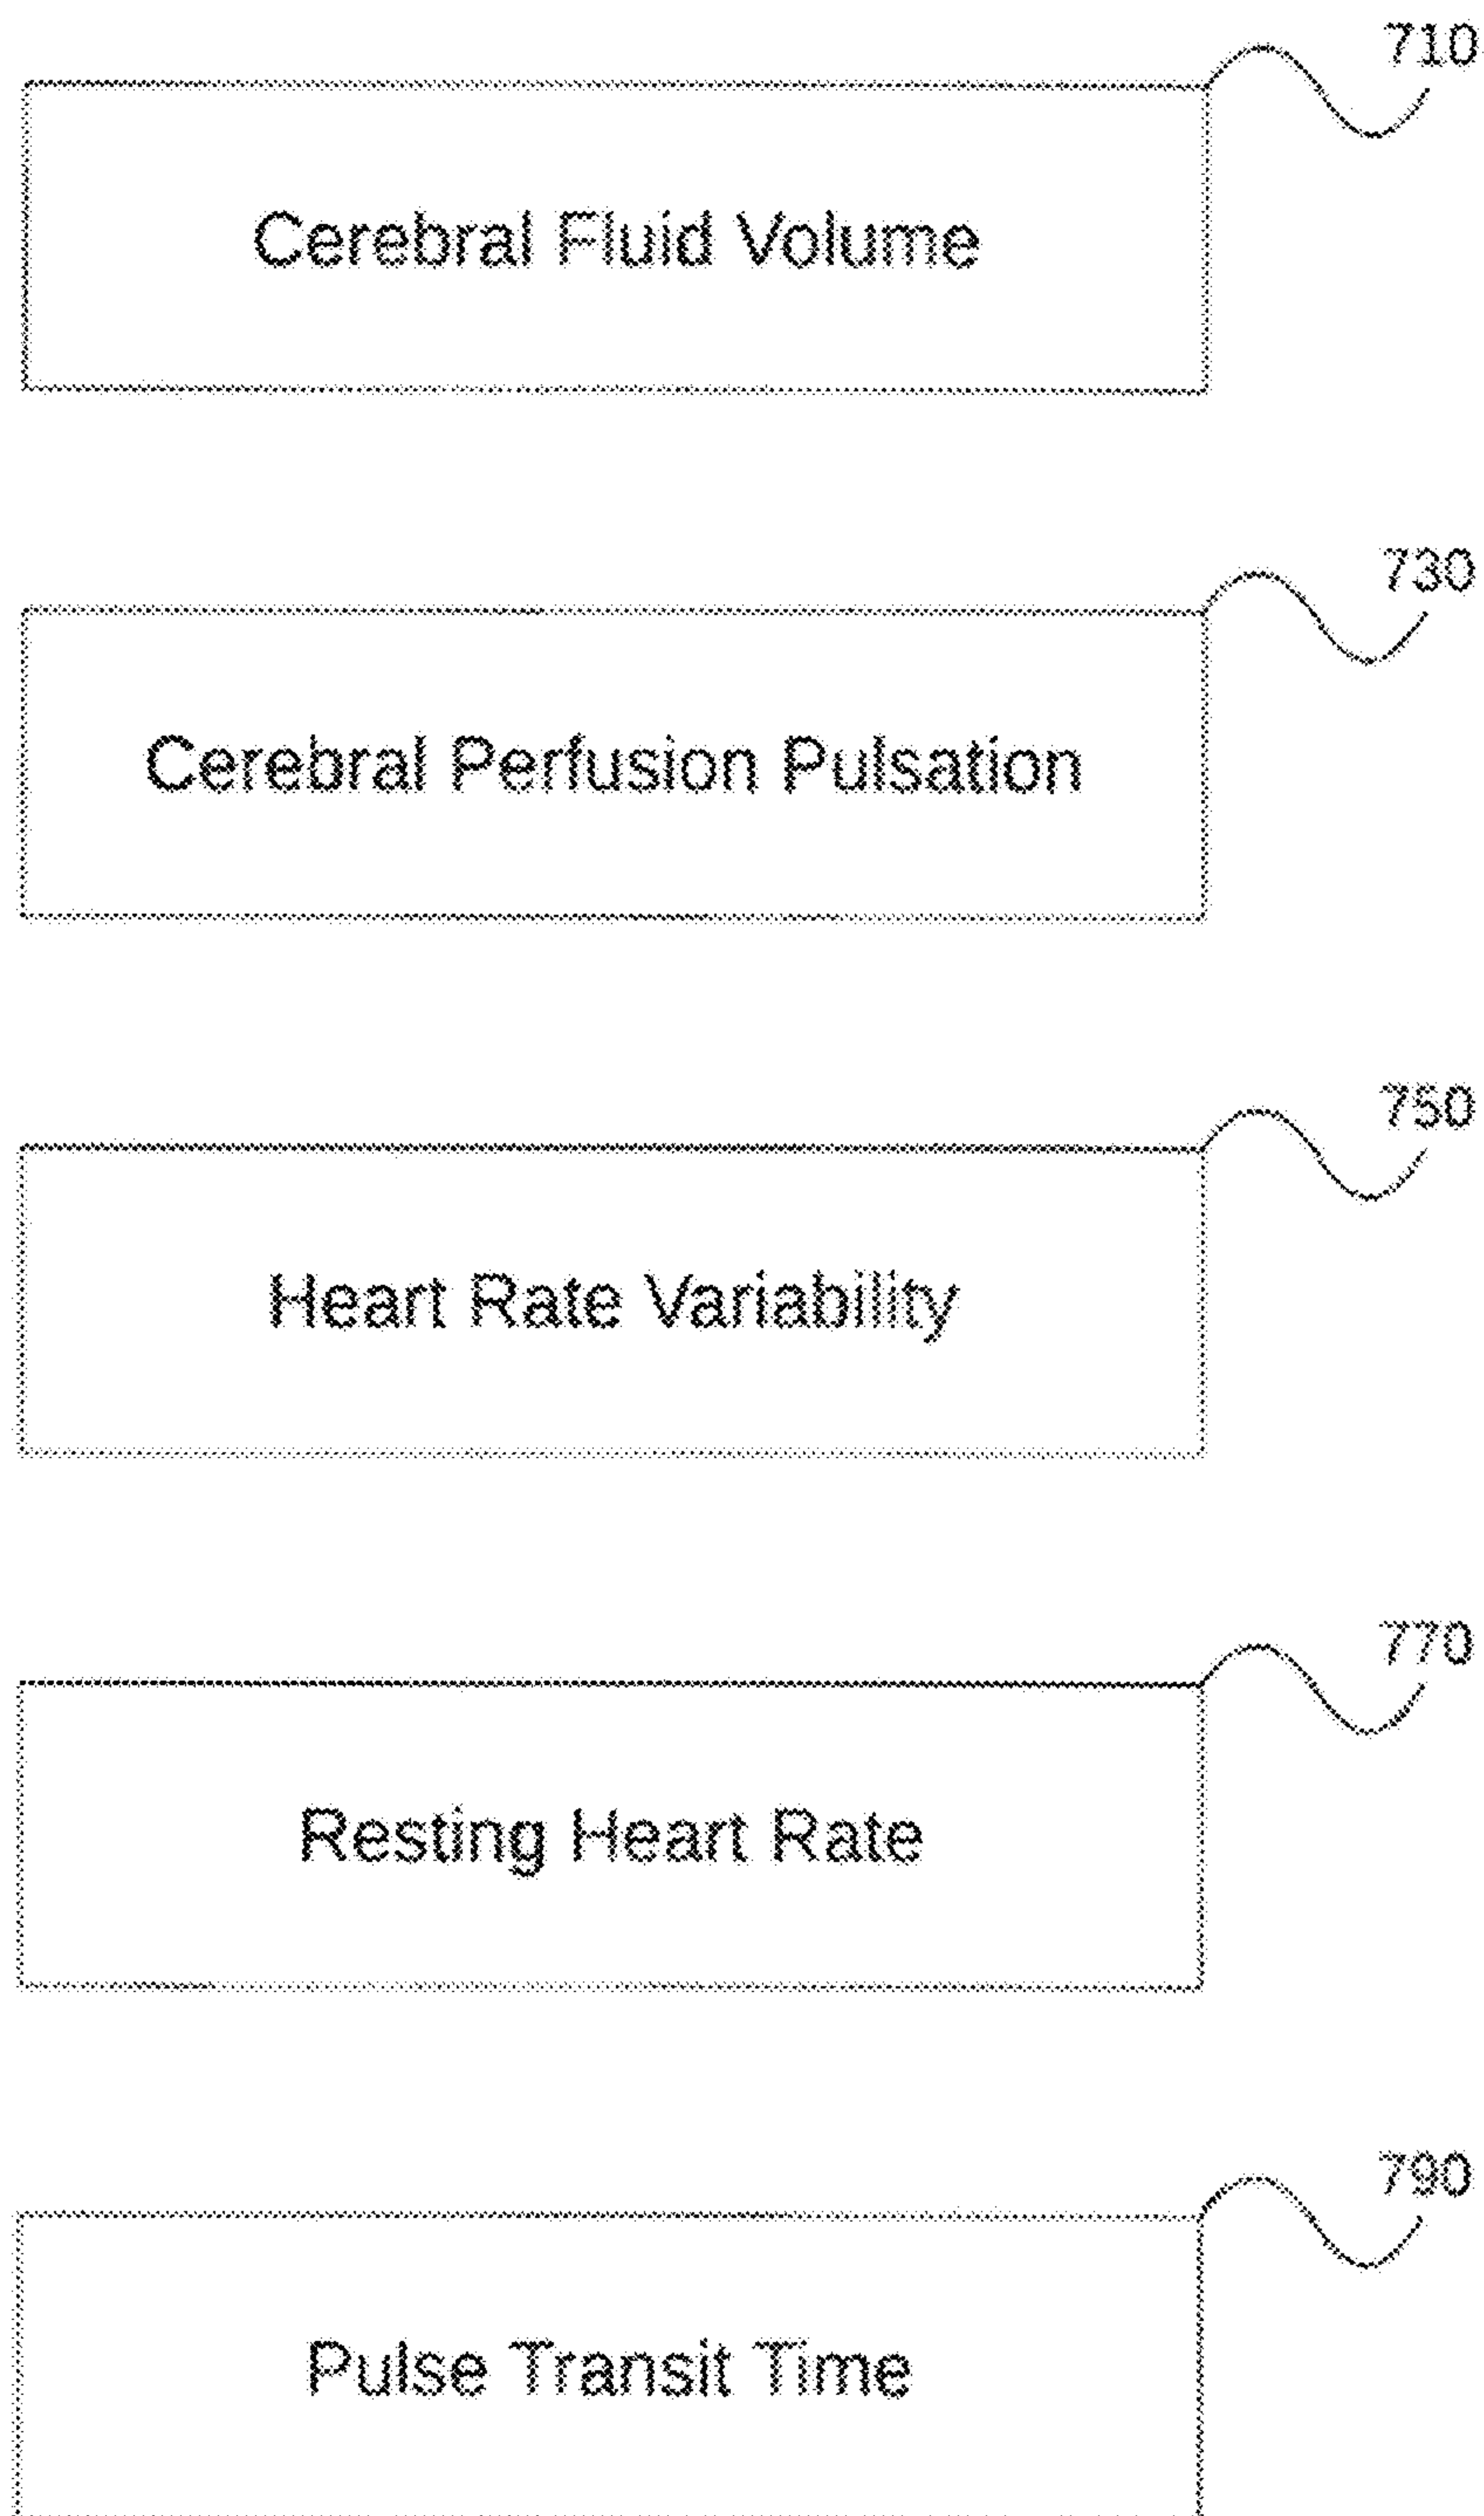
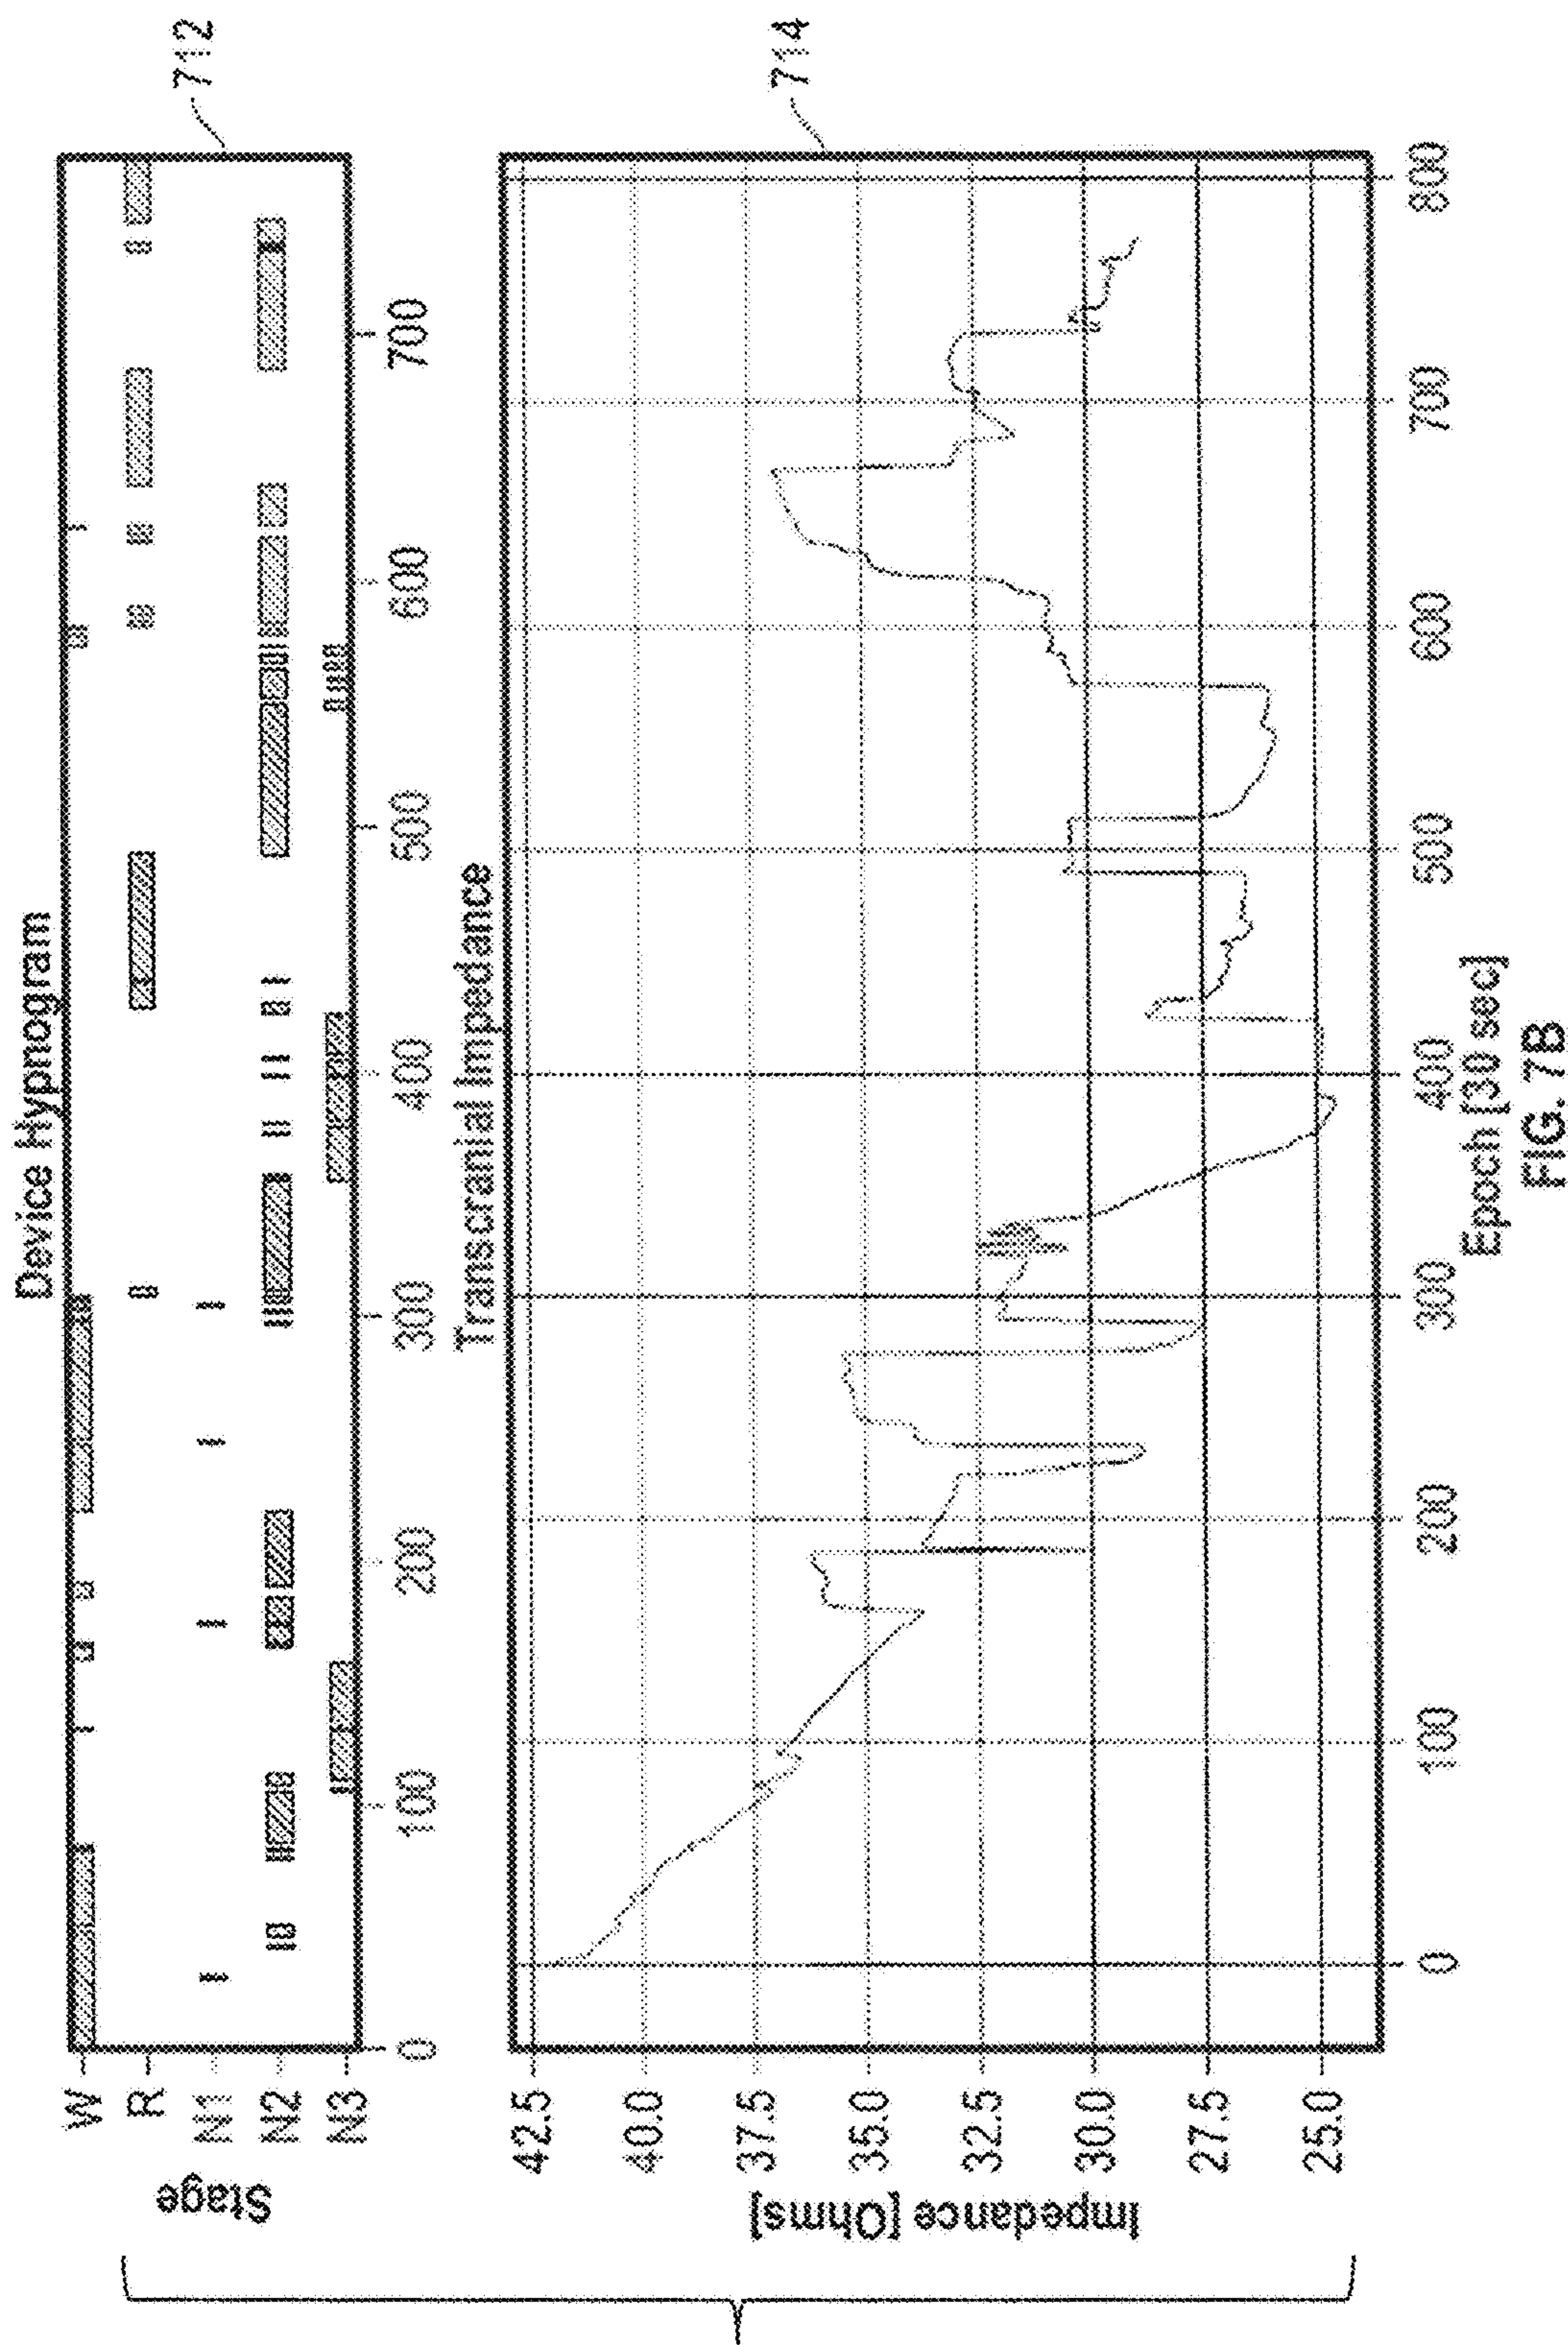


FIG. 7A



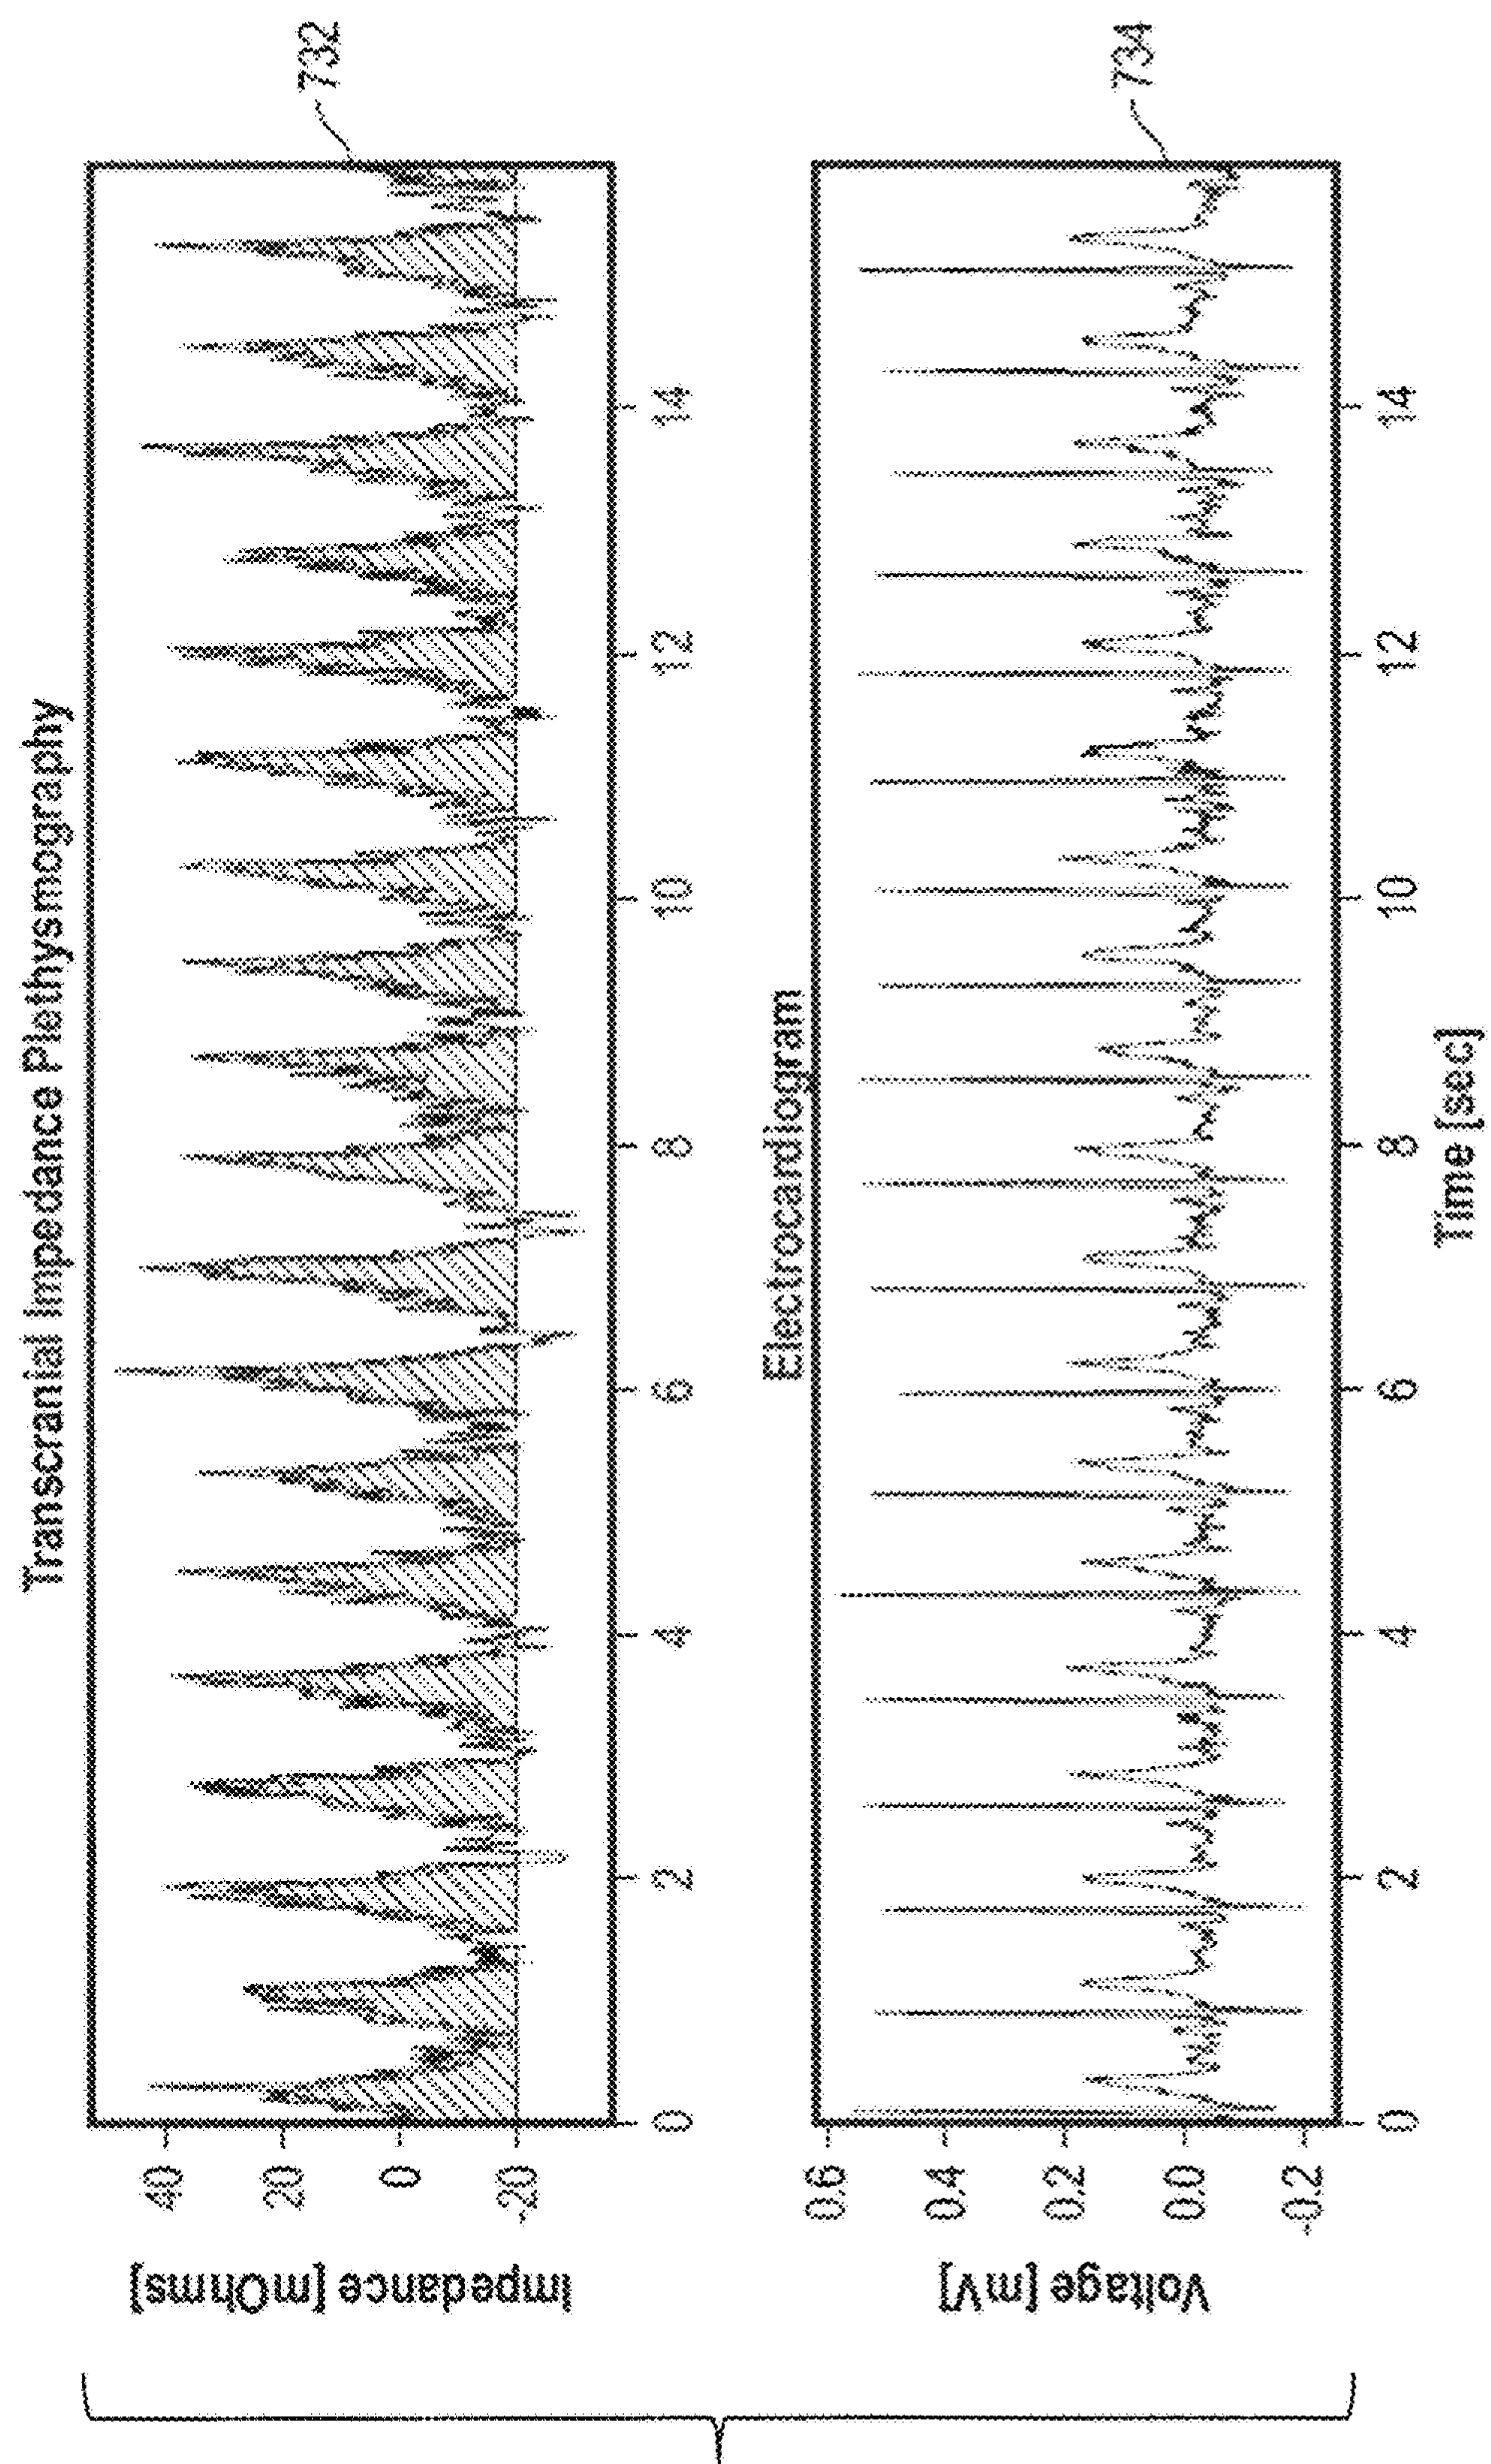


FIG. 7B cont.

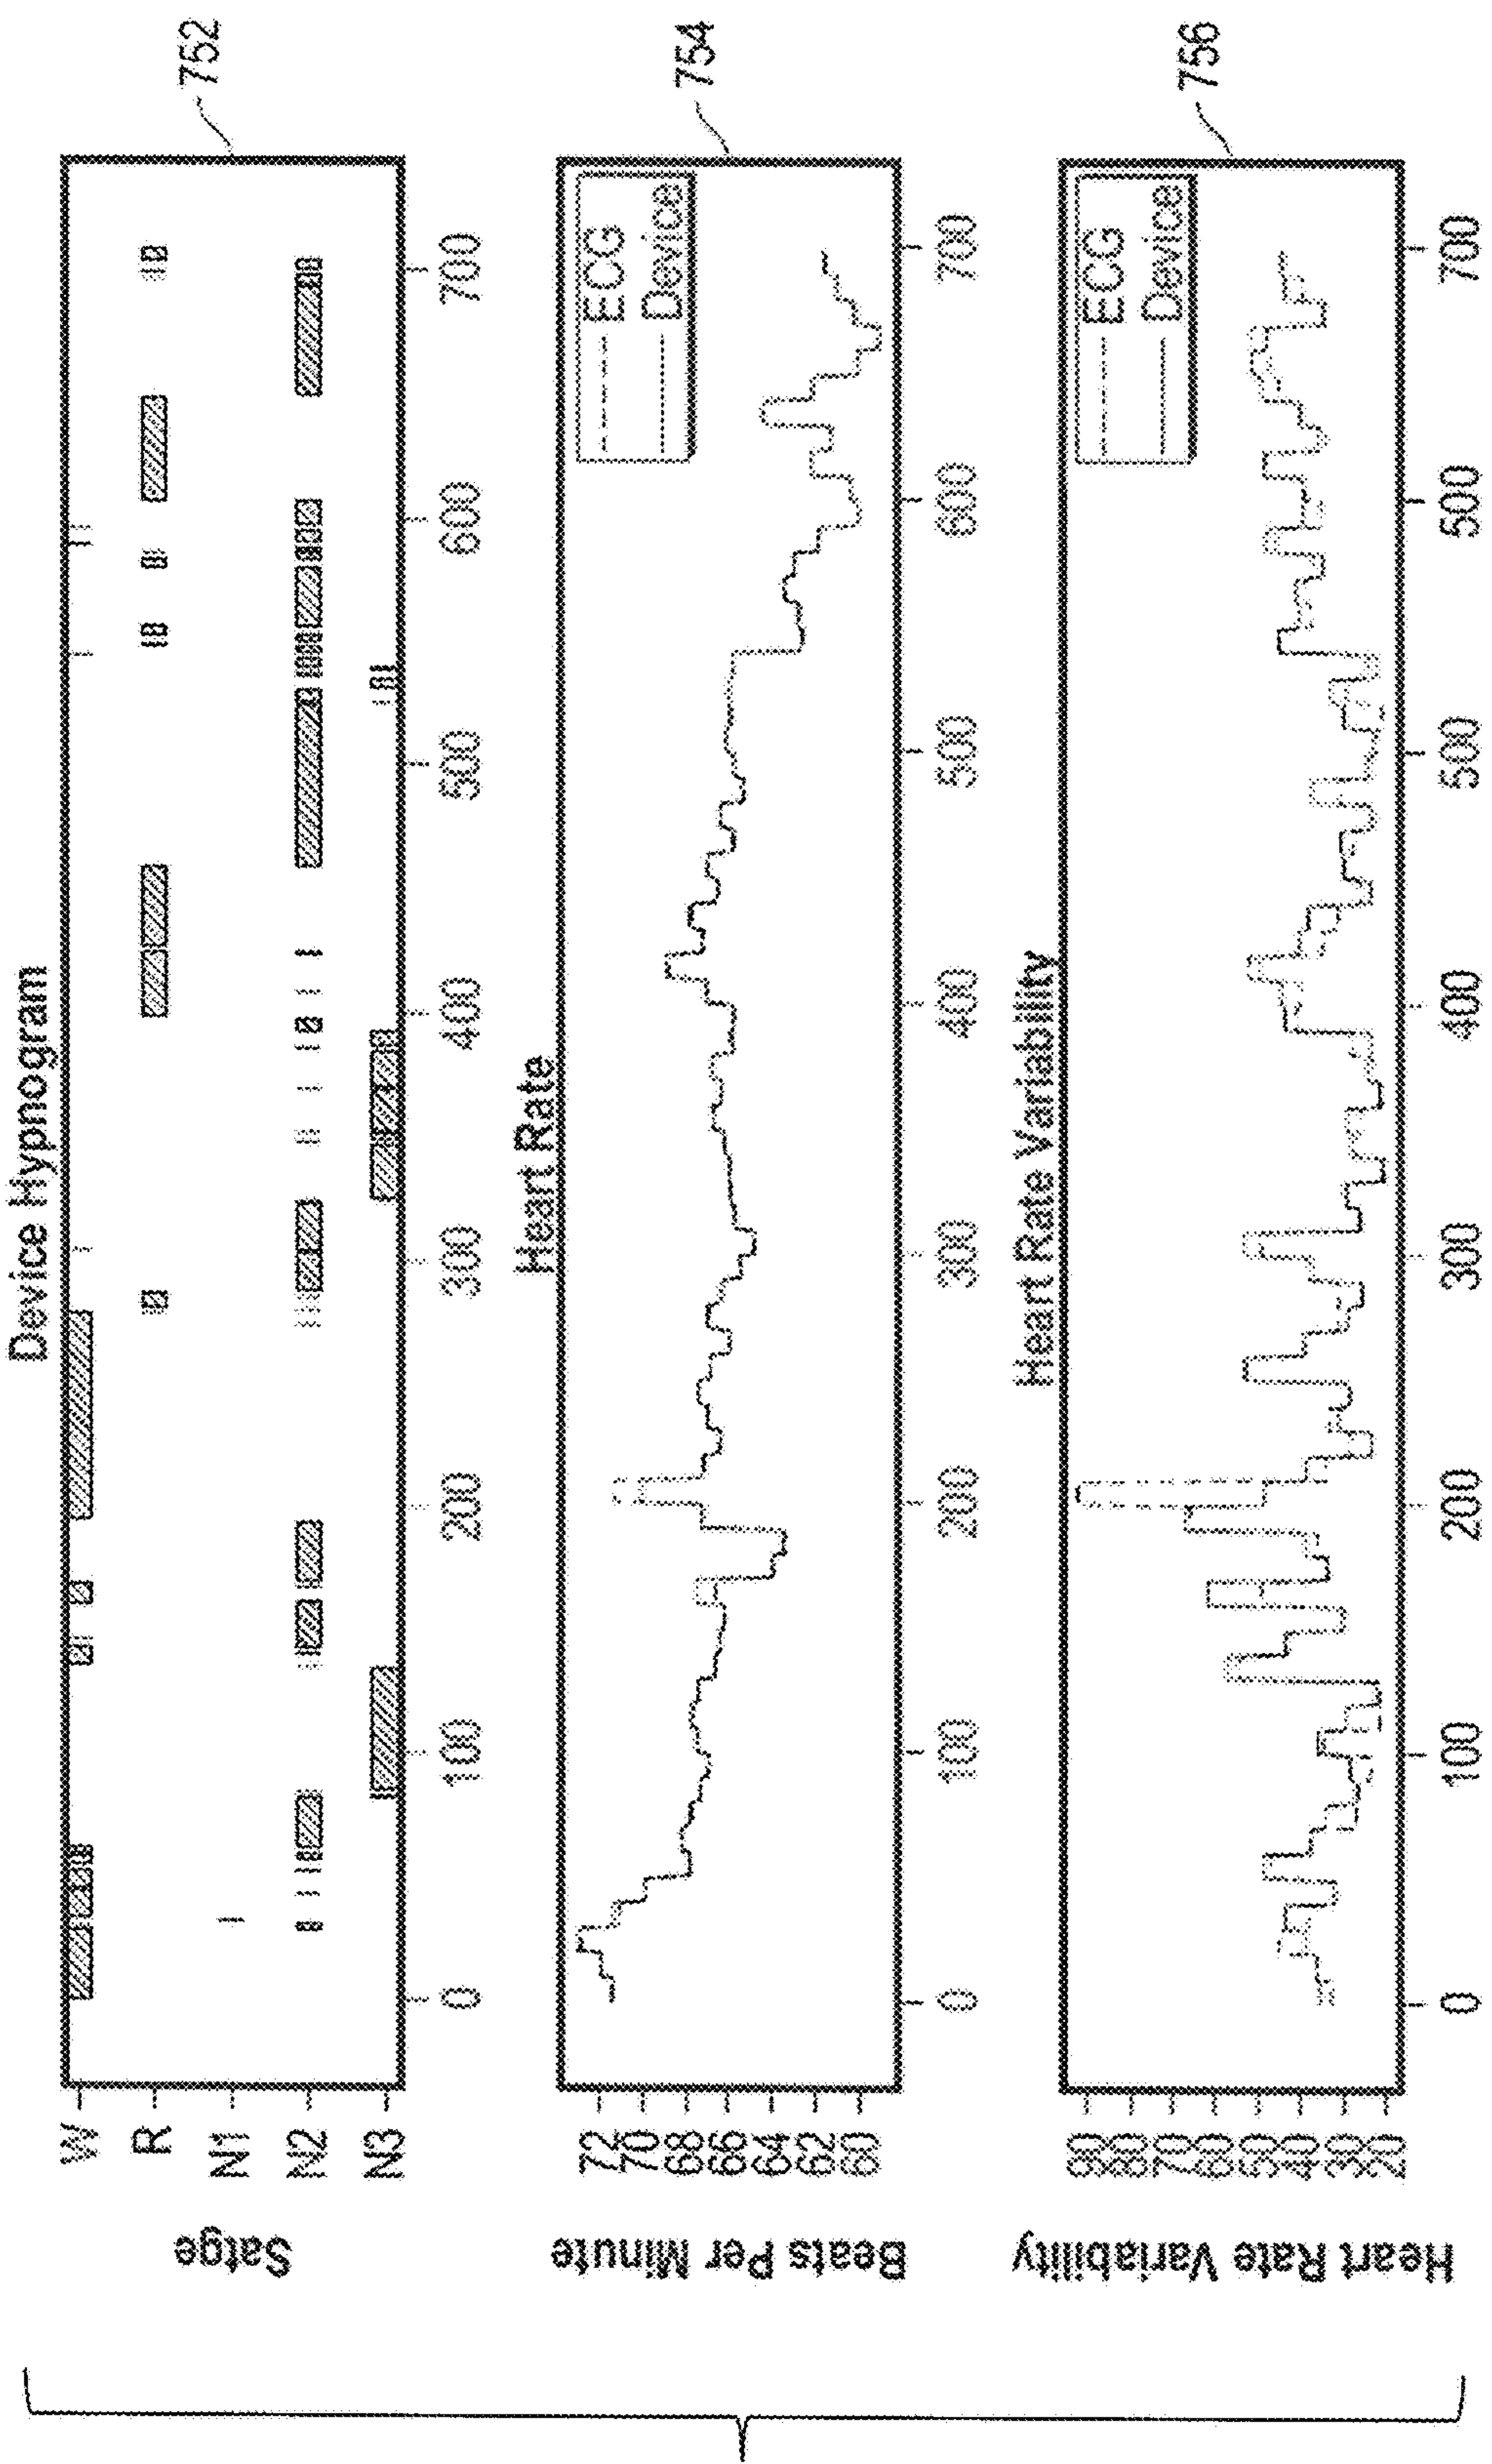


FIG. 7C

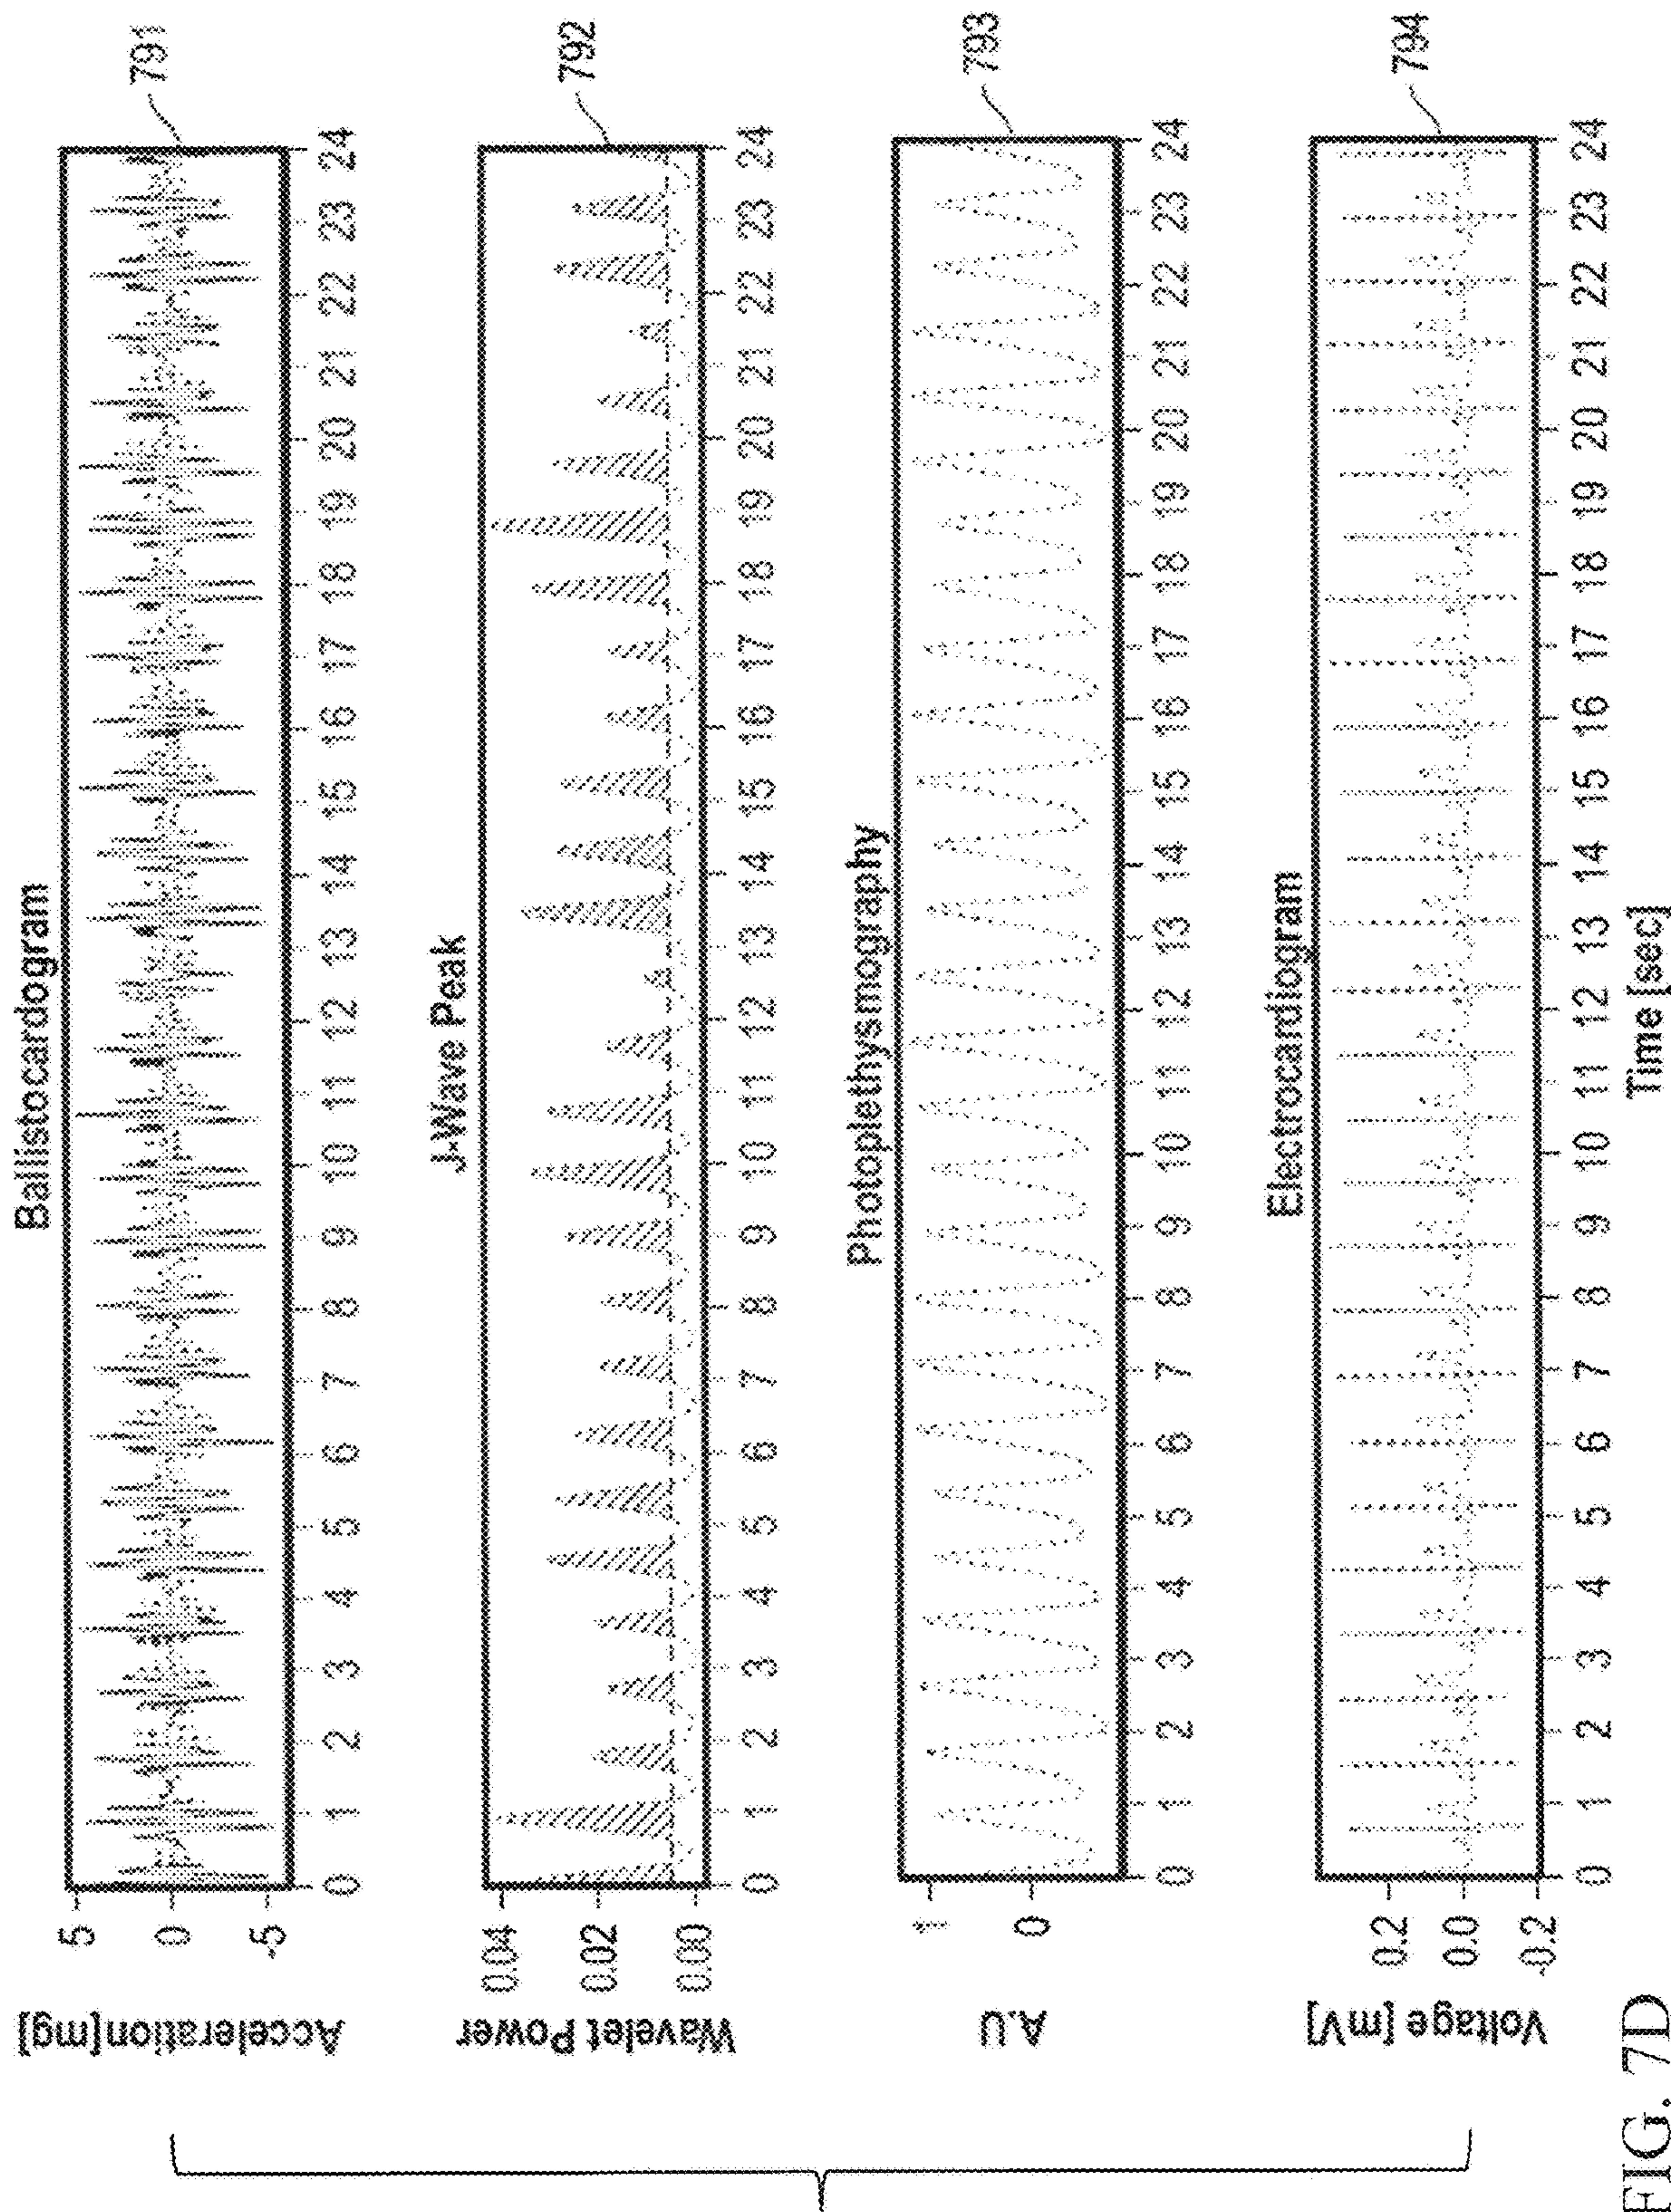
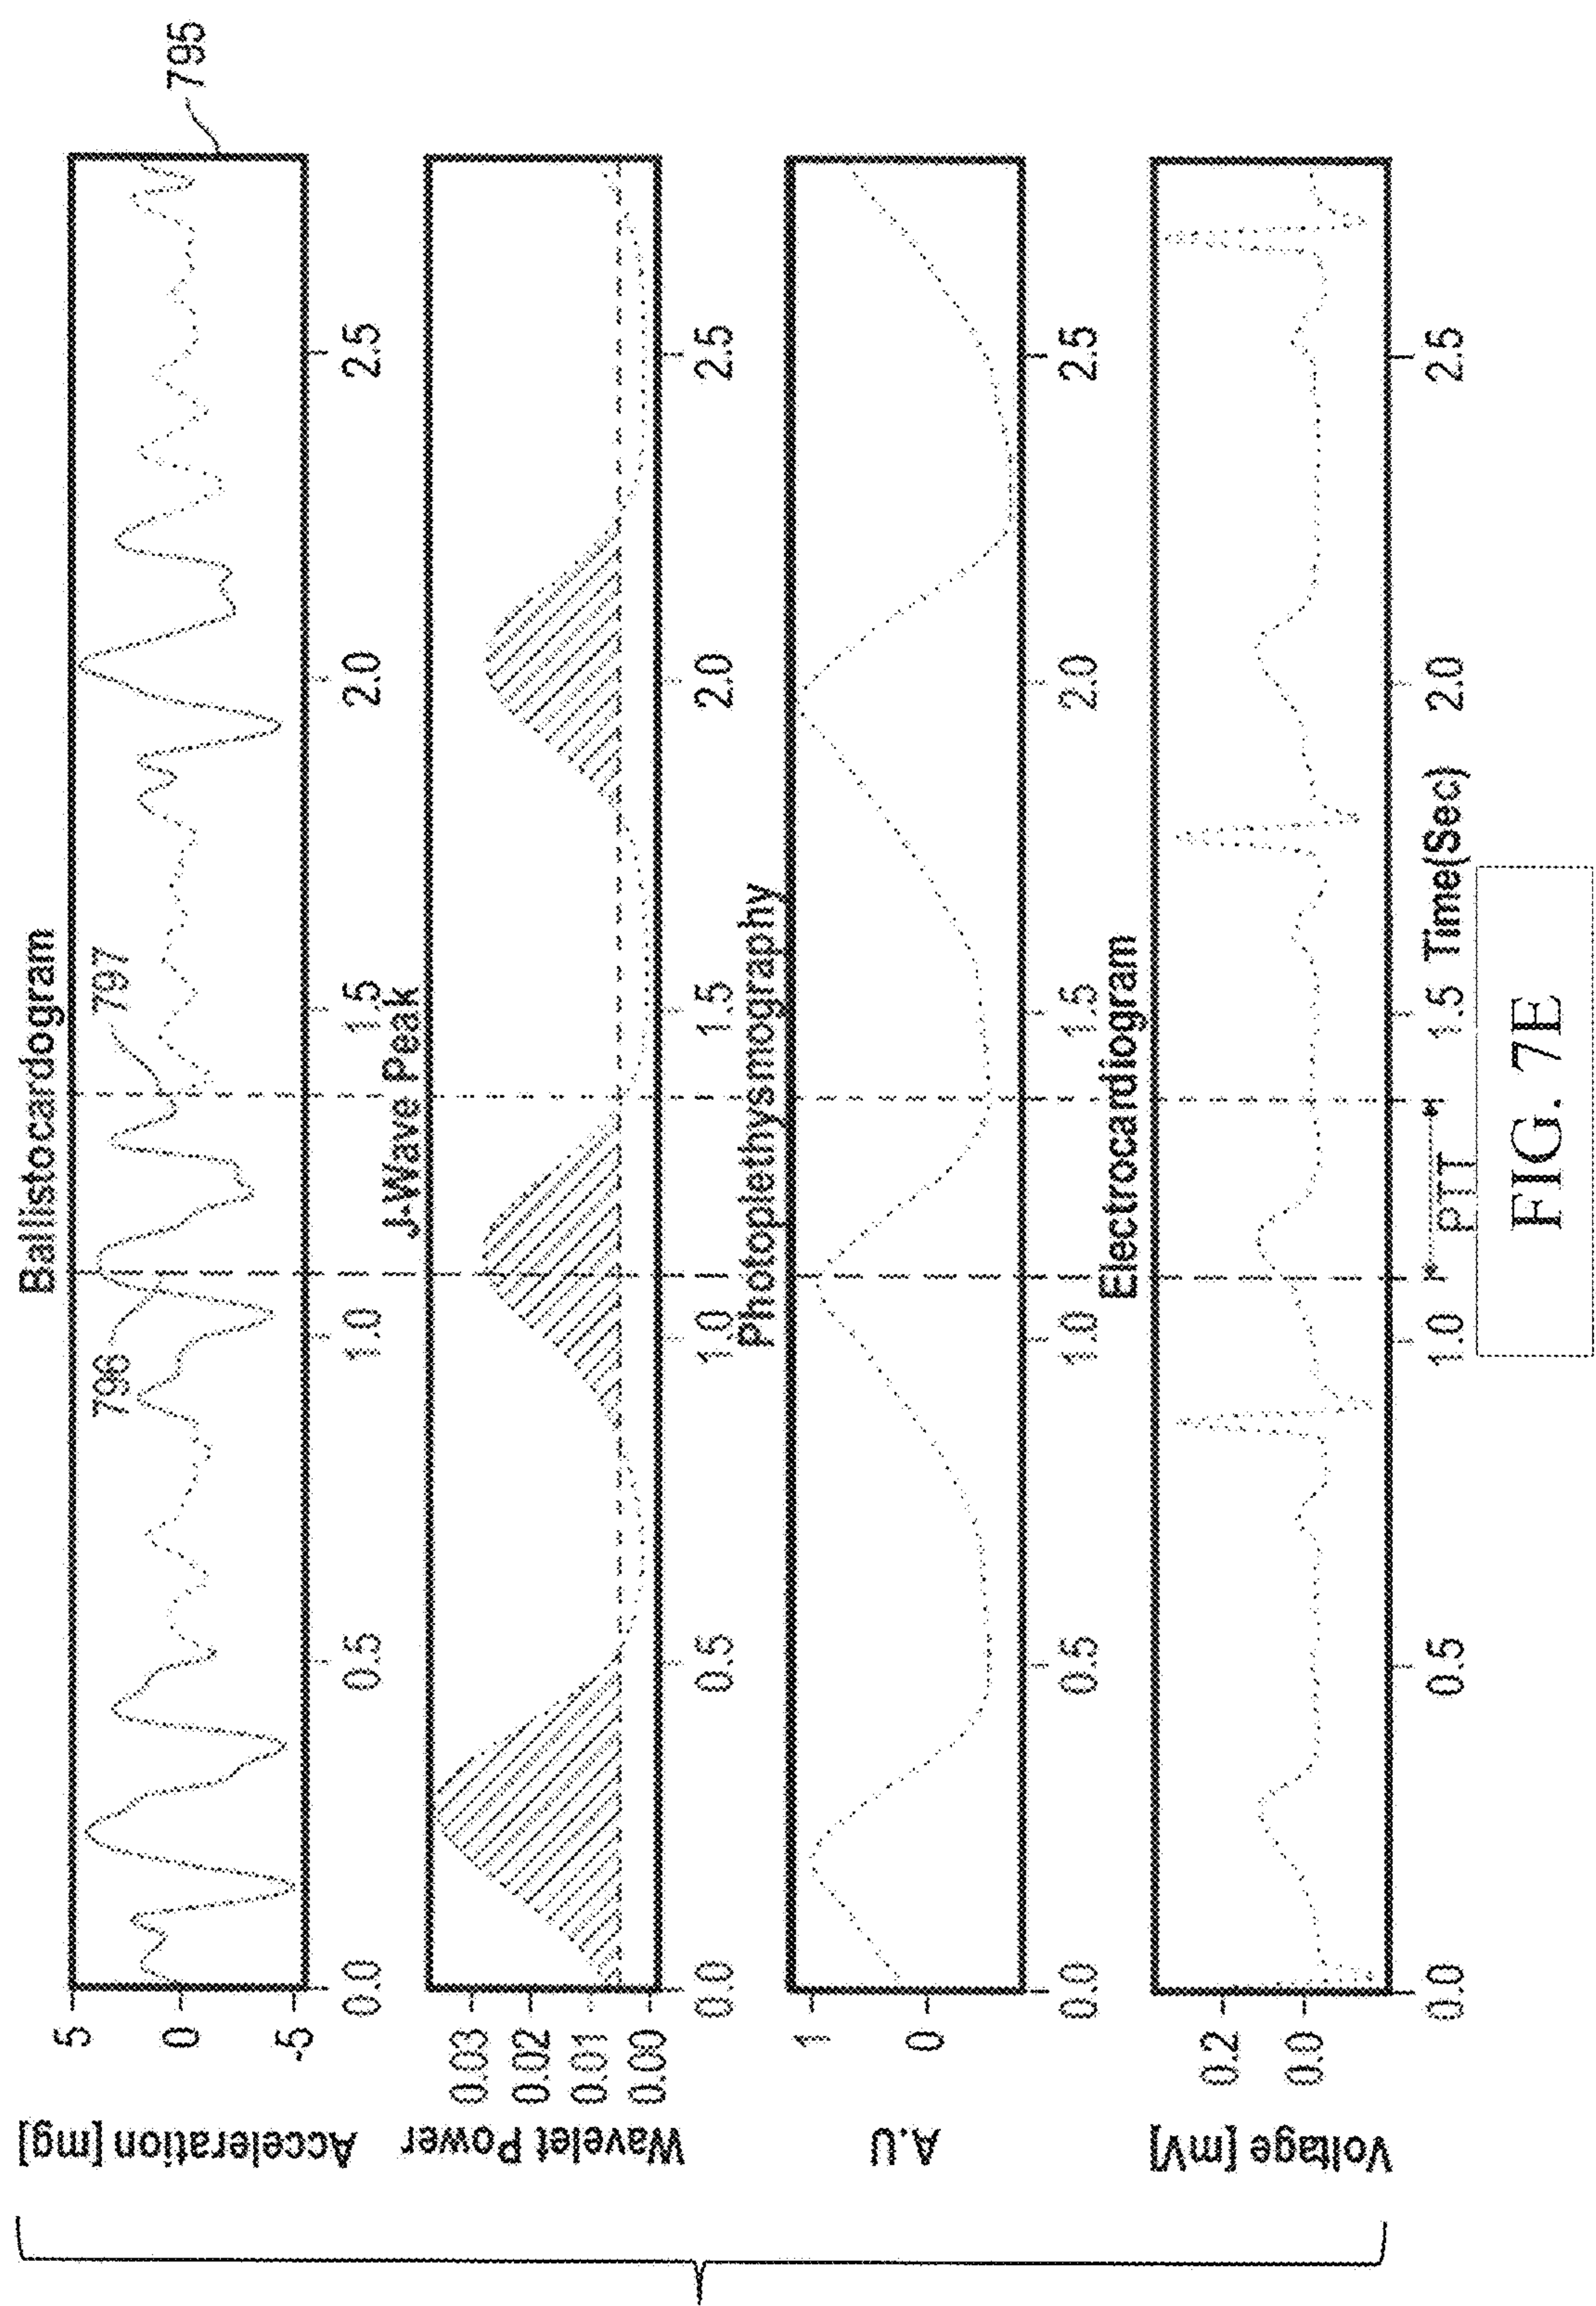


FIG. 7D



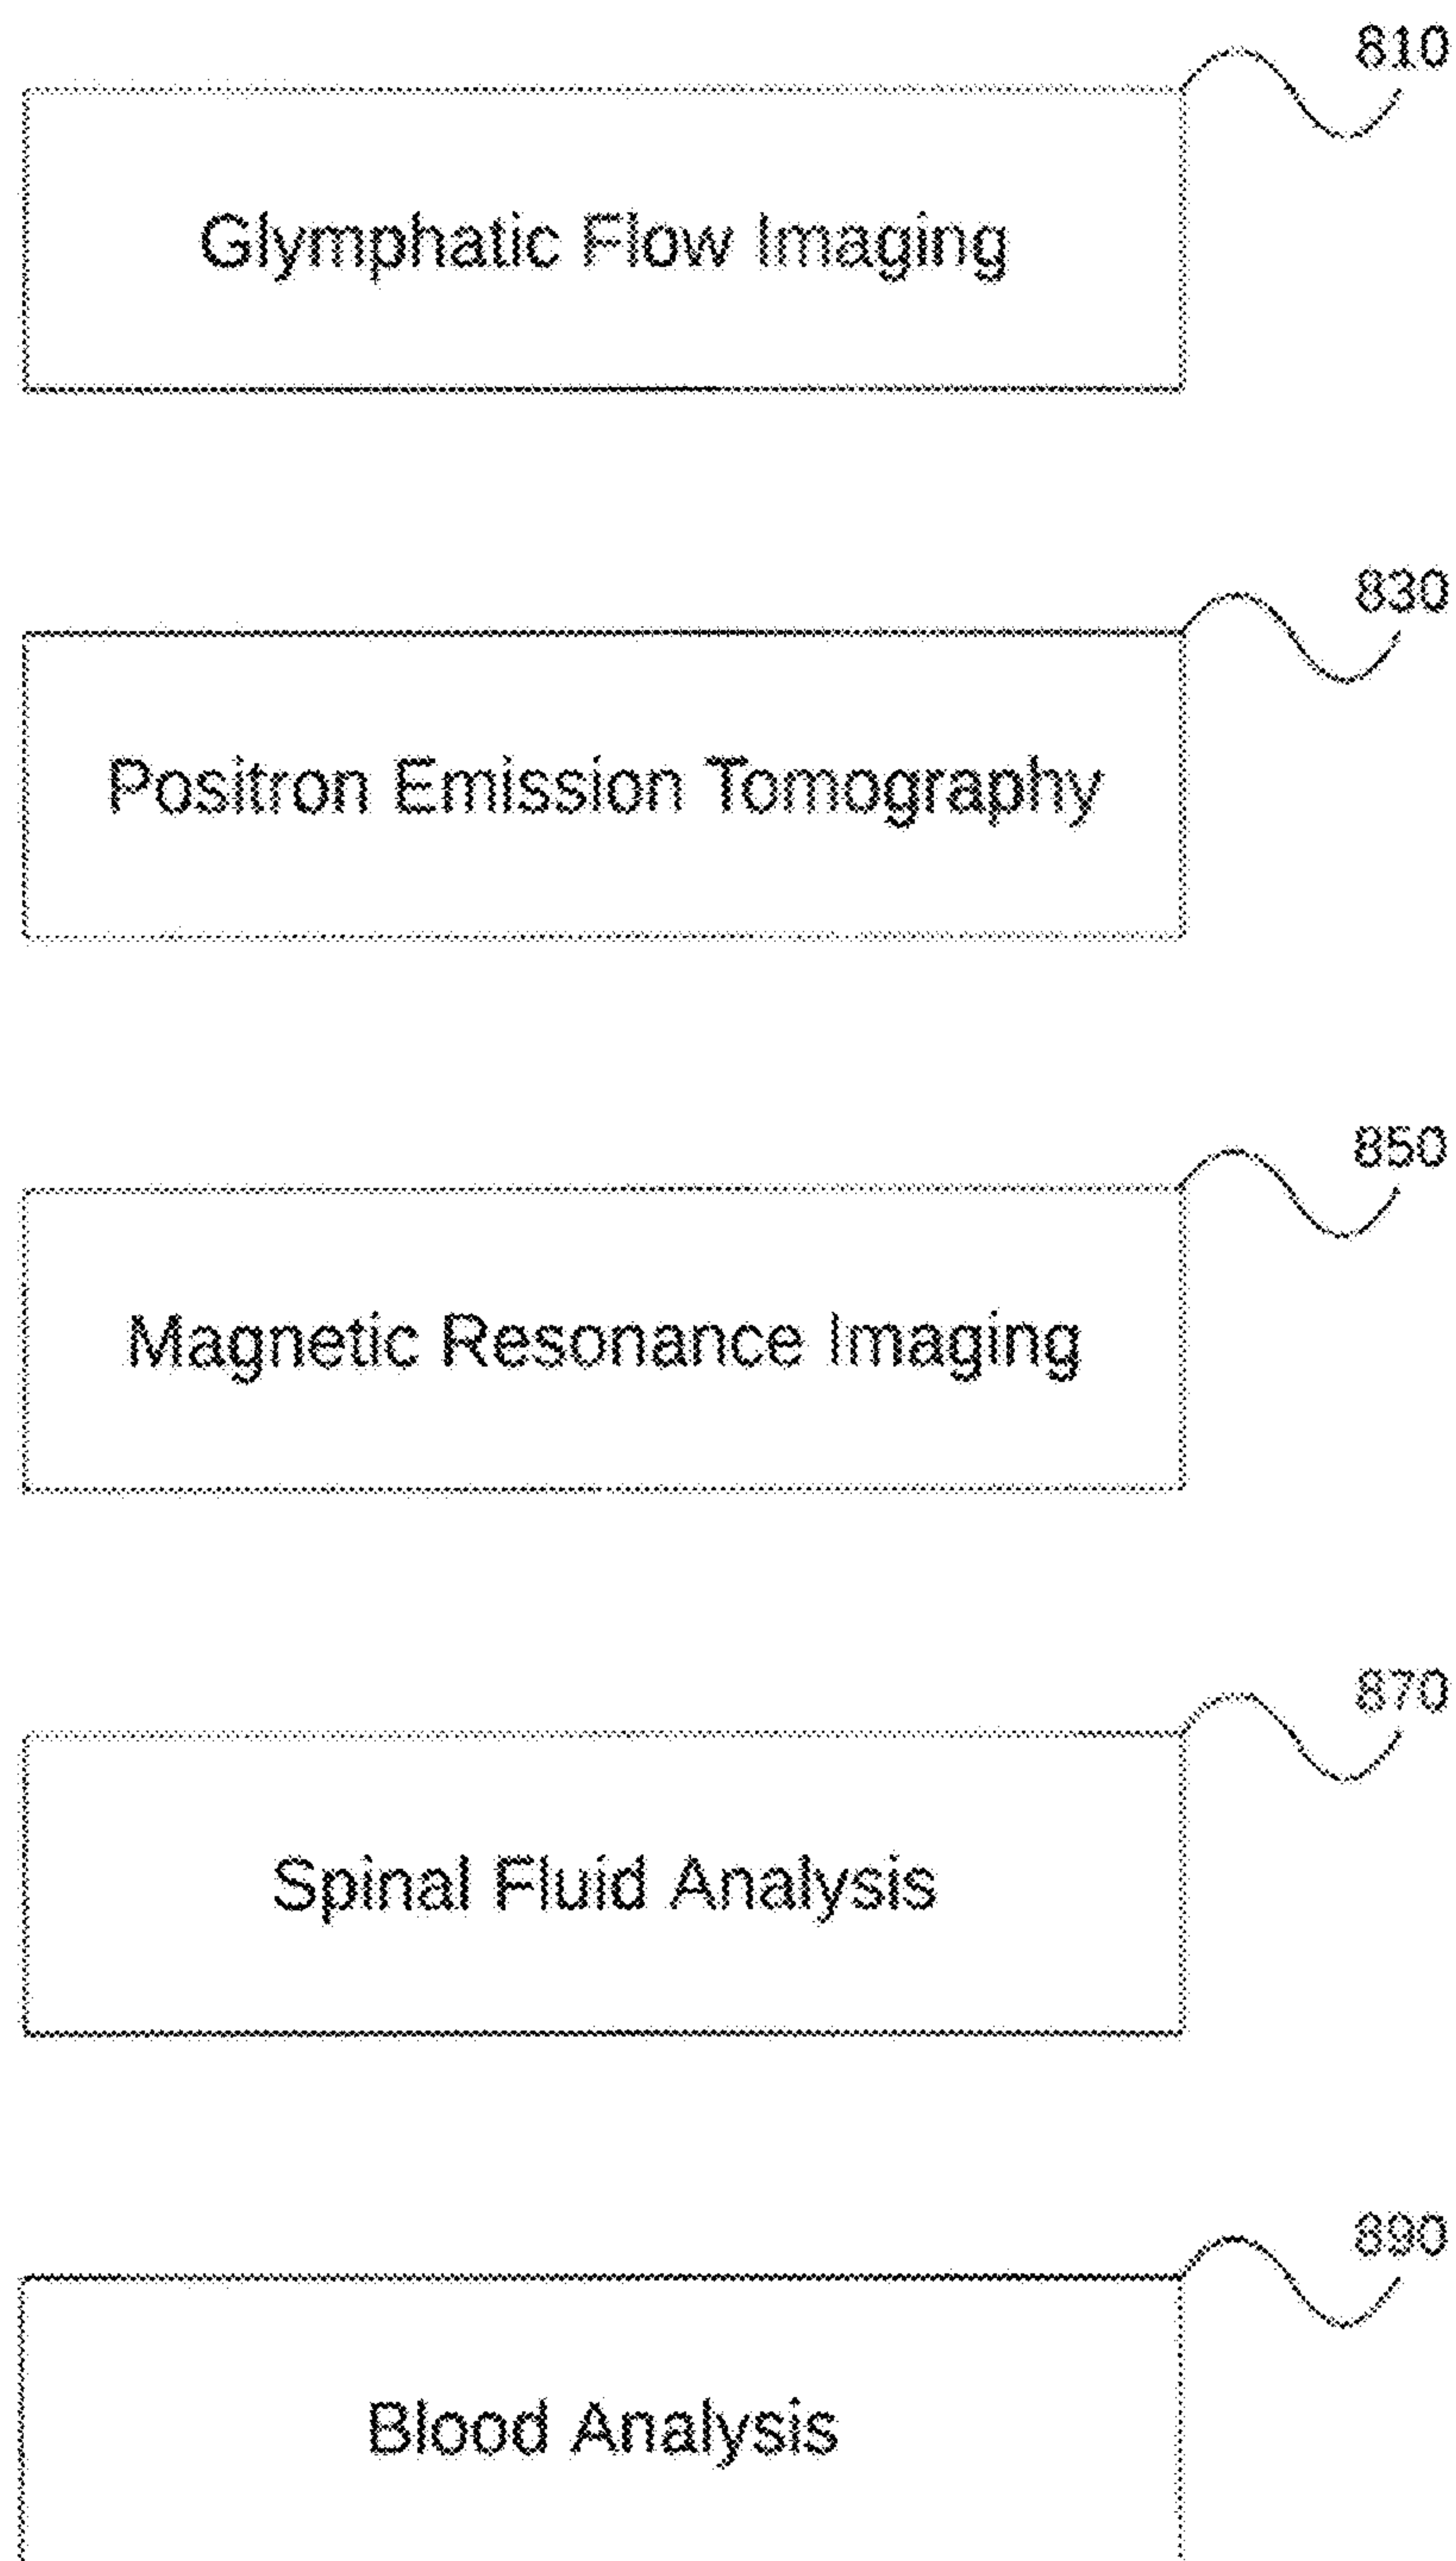


FIG. 8A

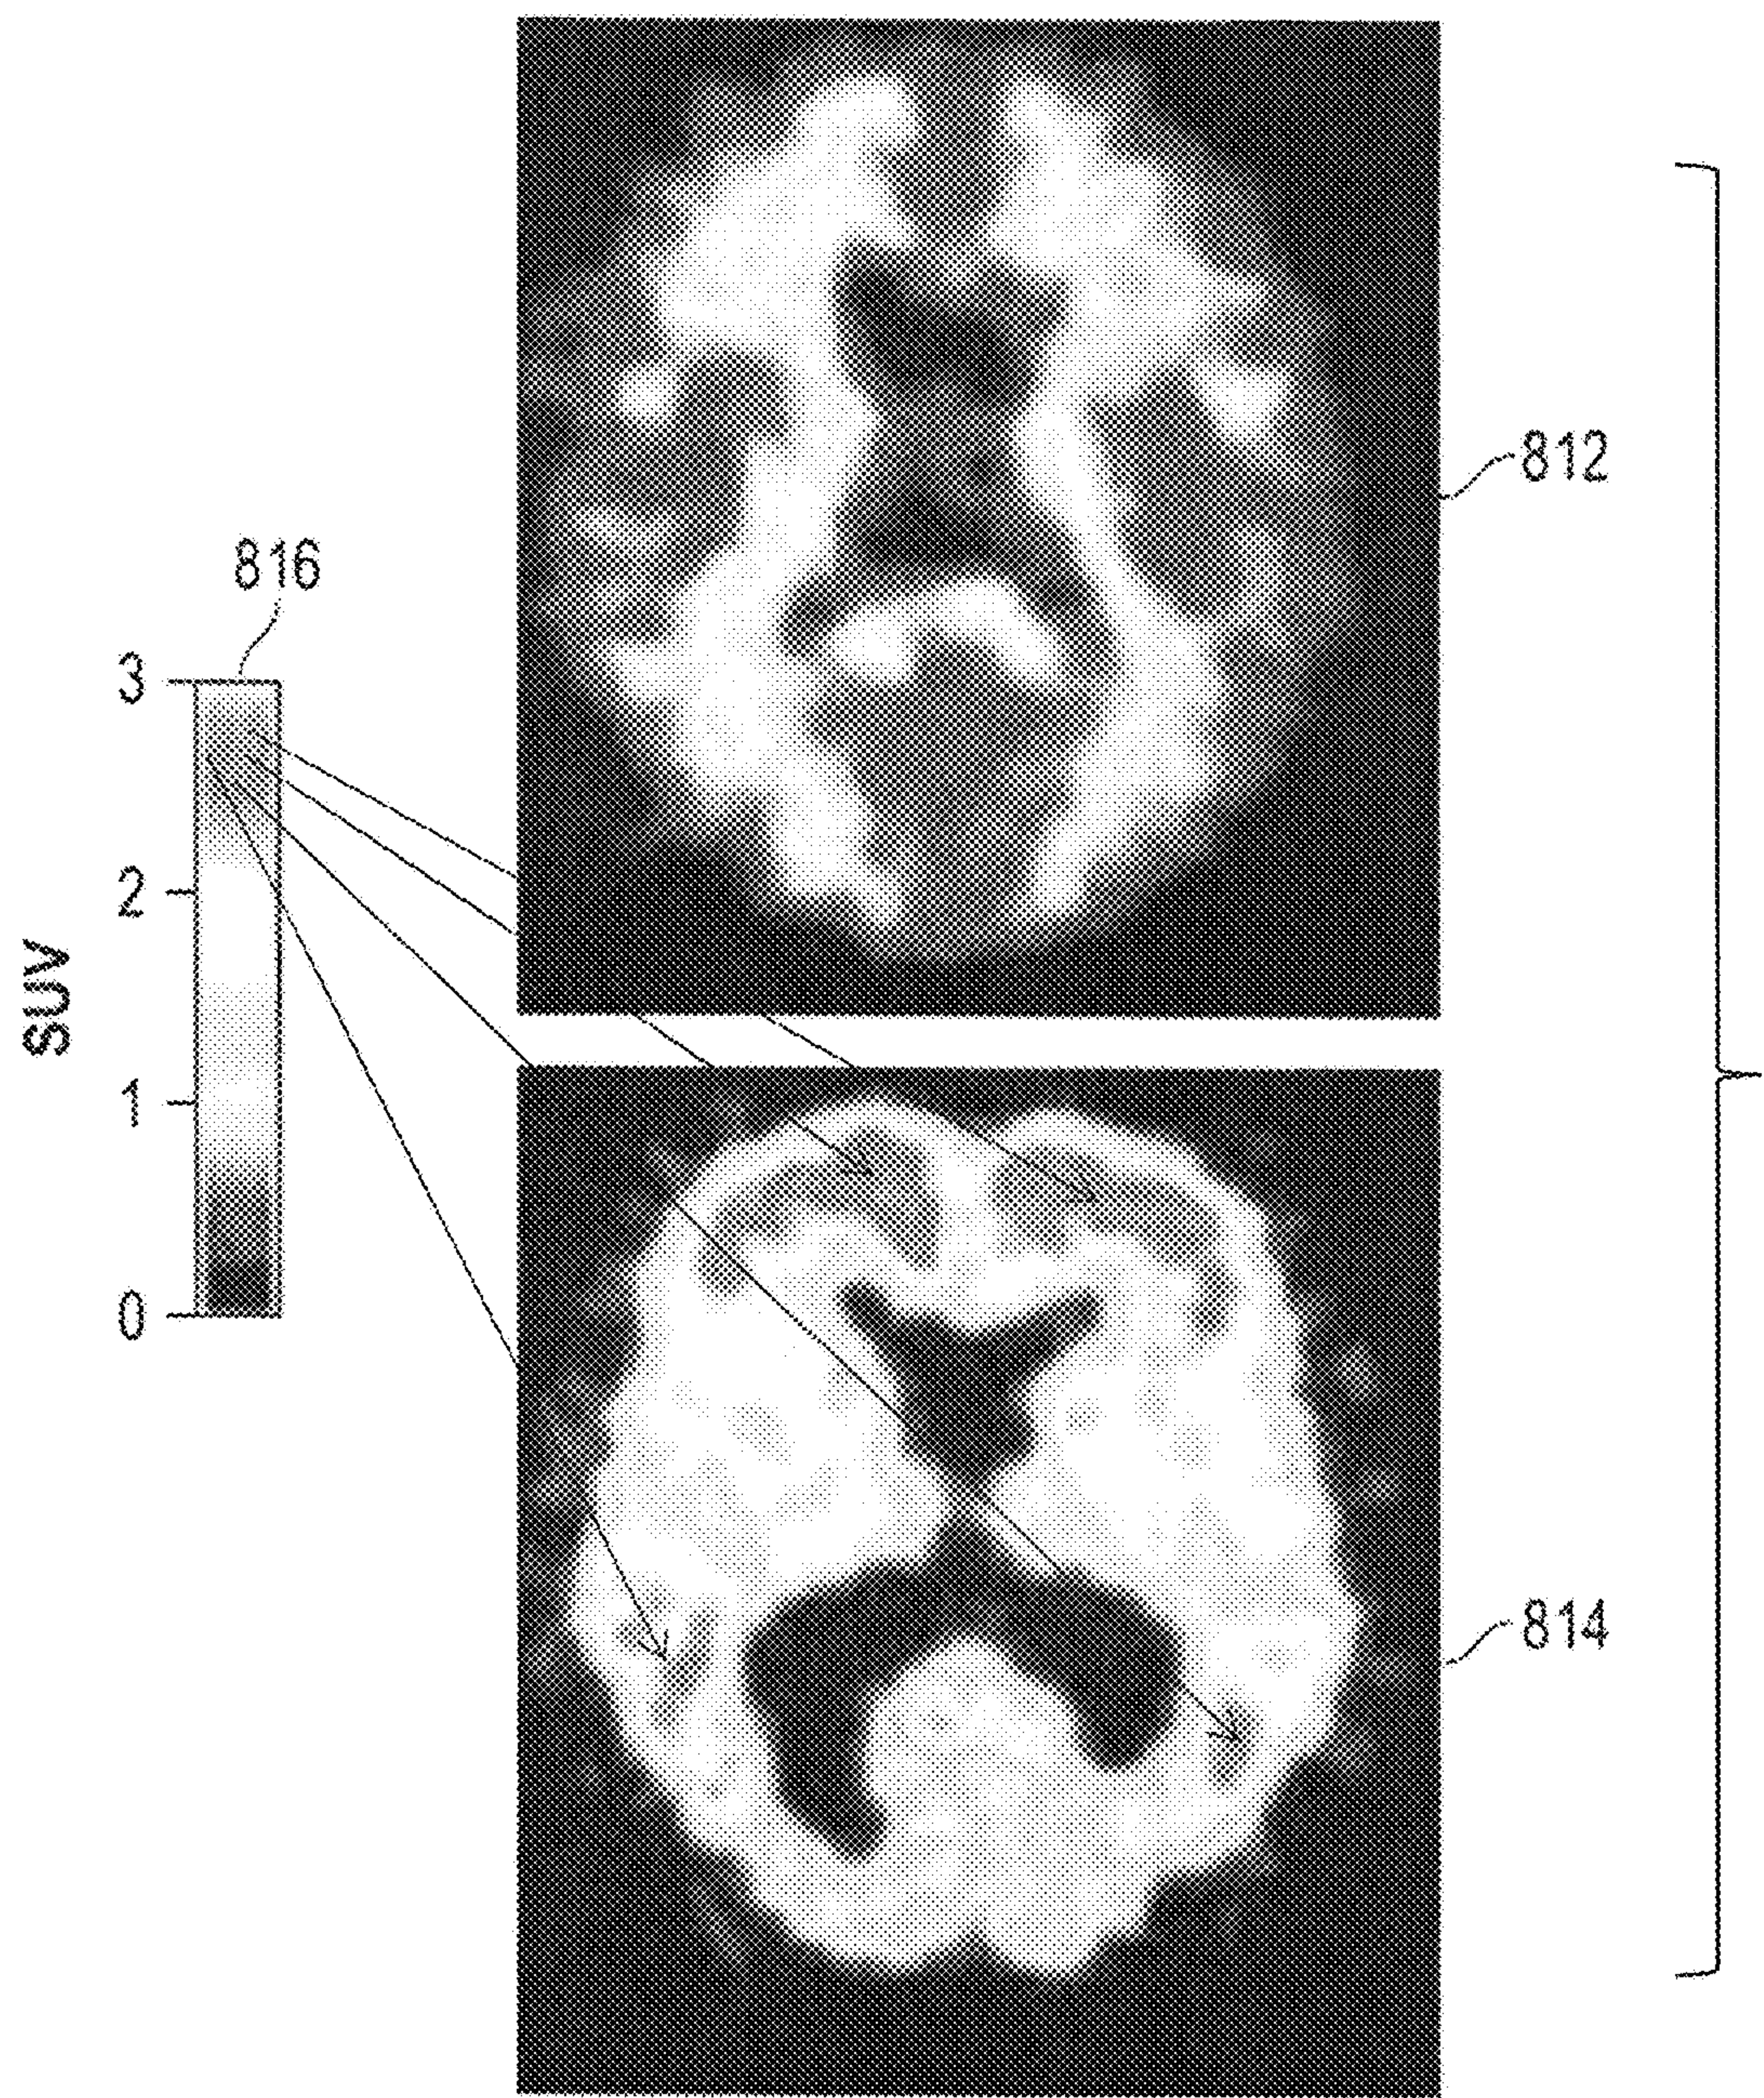


FIG. 8B

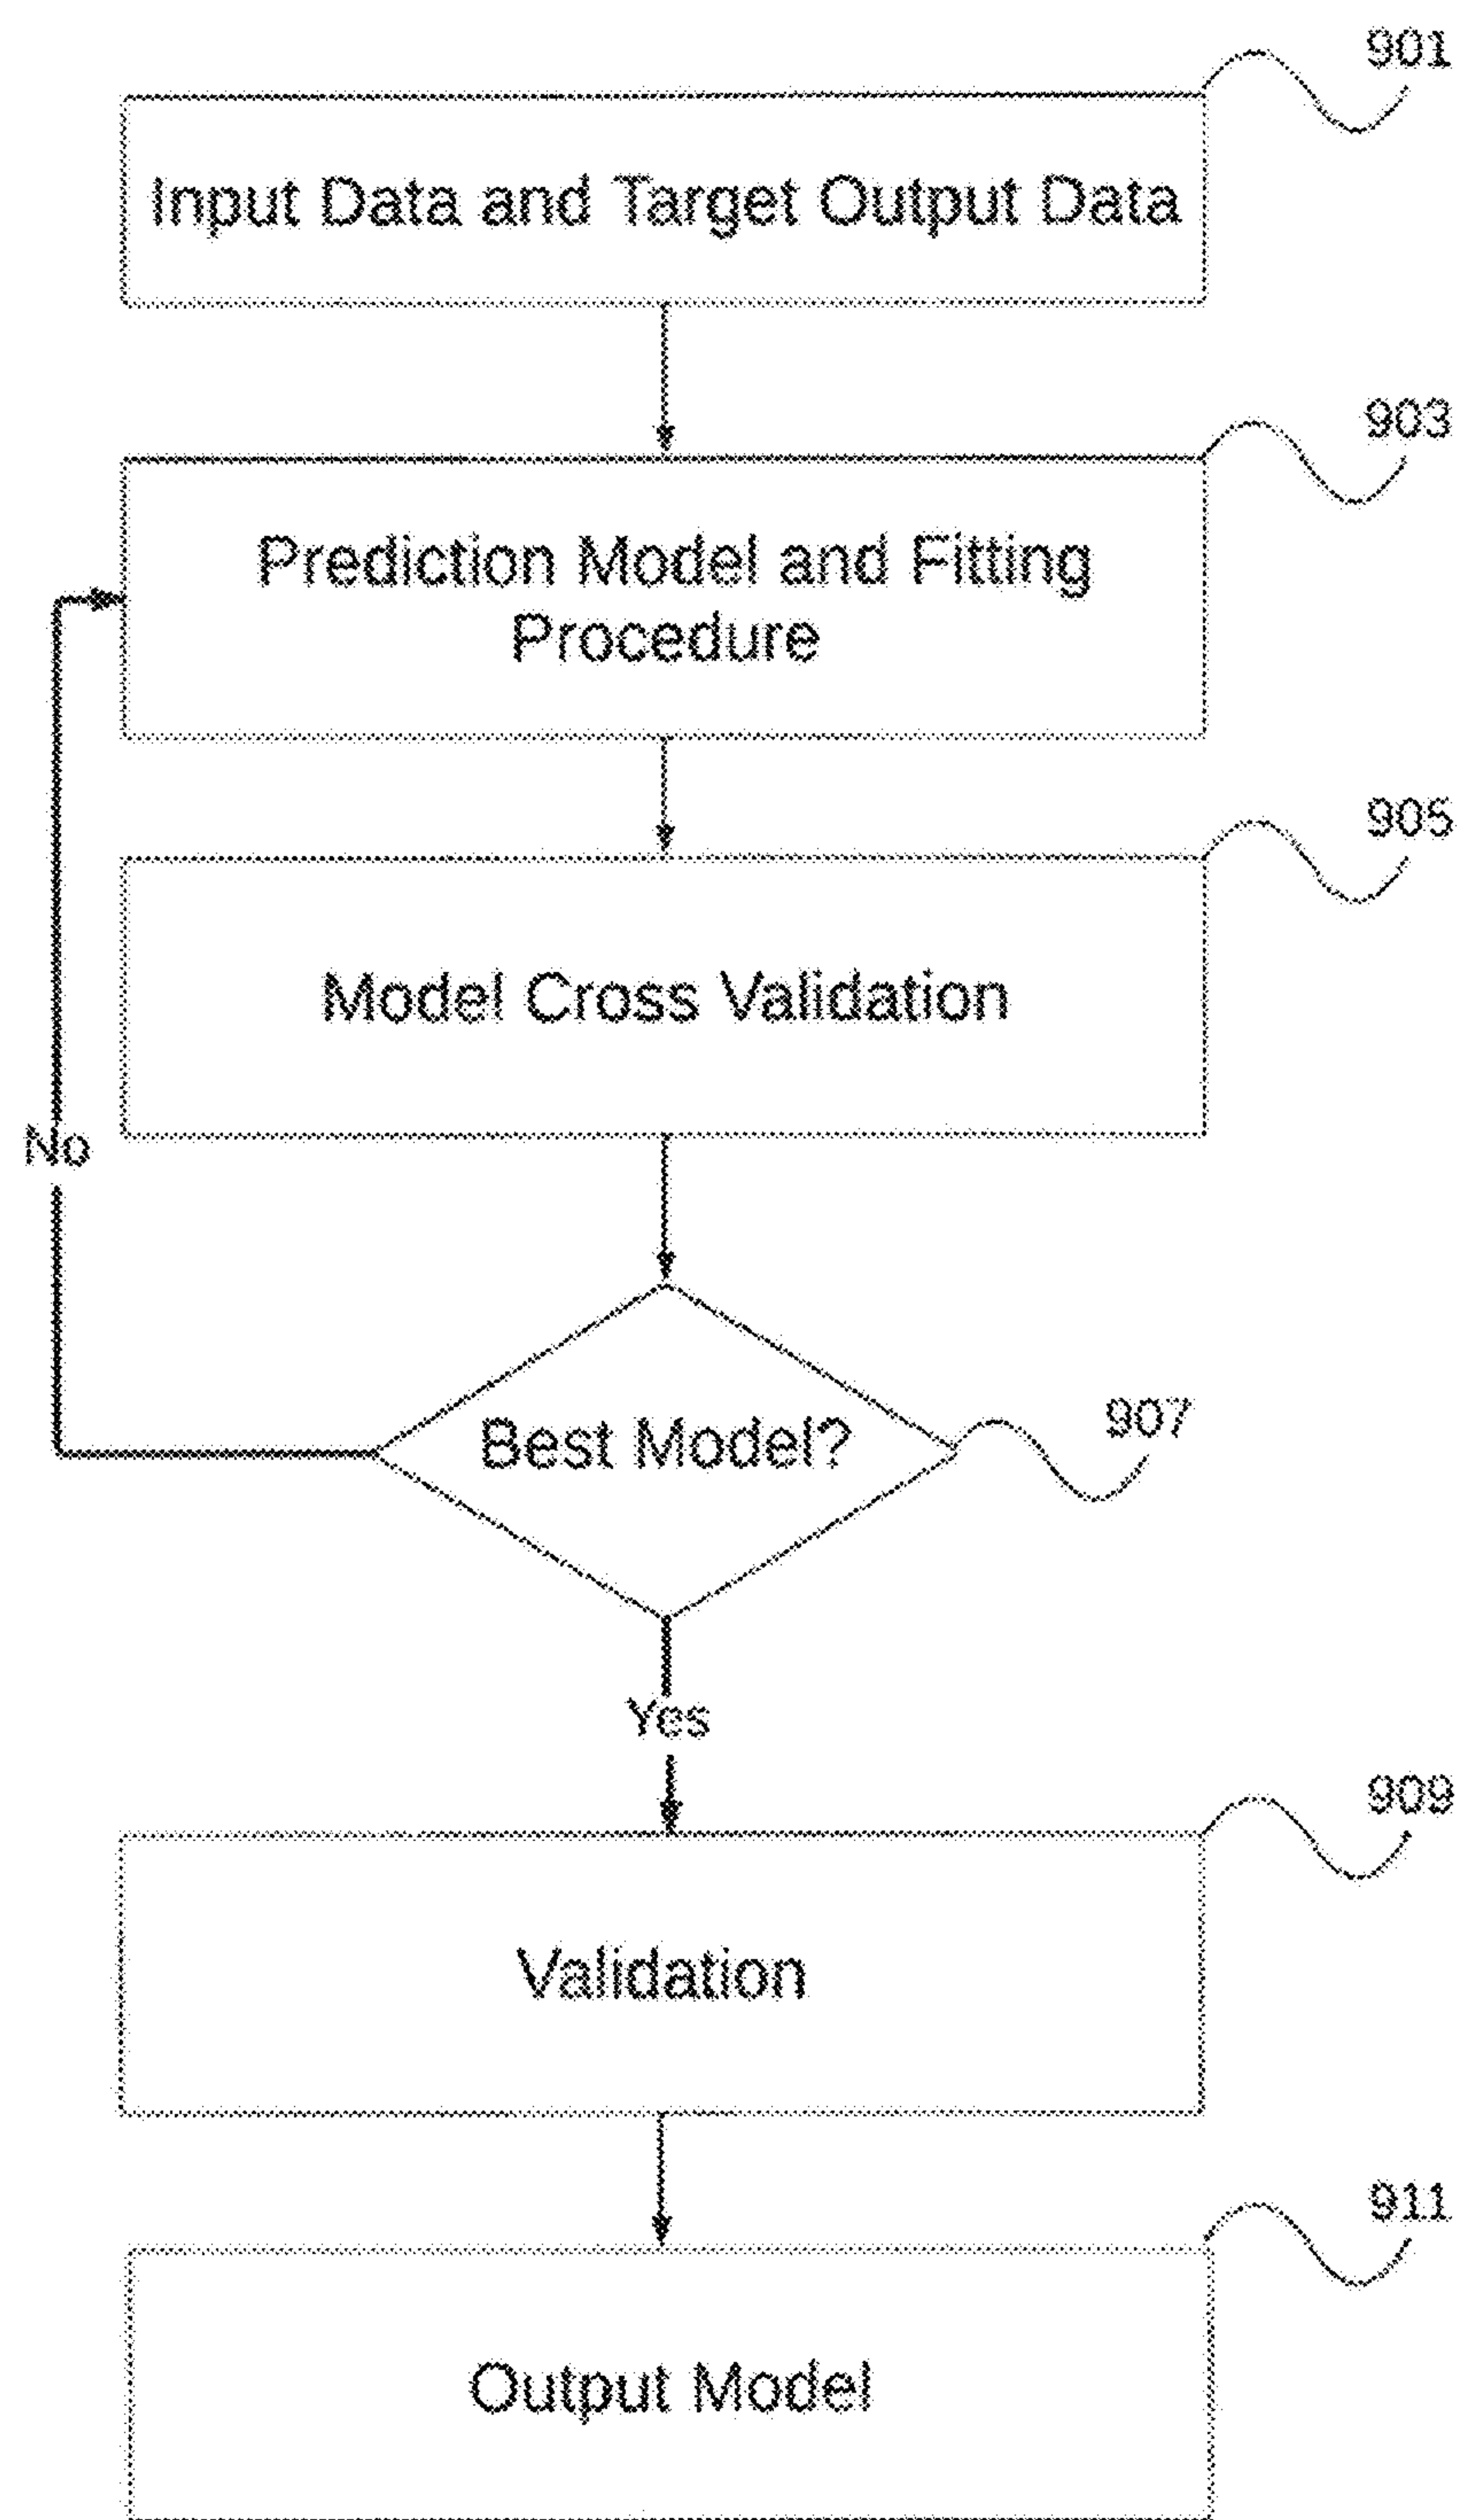


FIG. 9

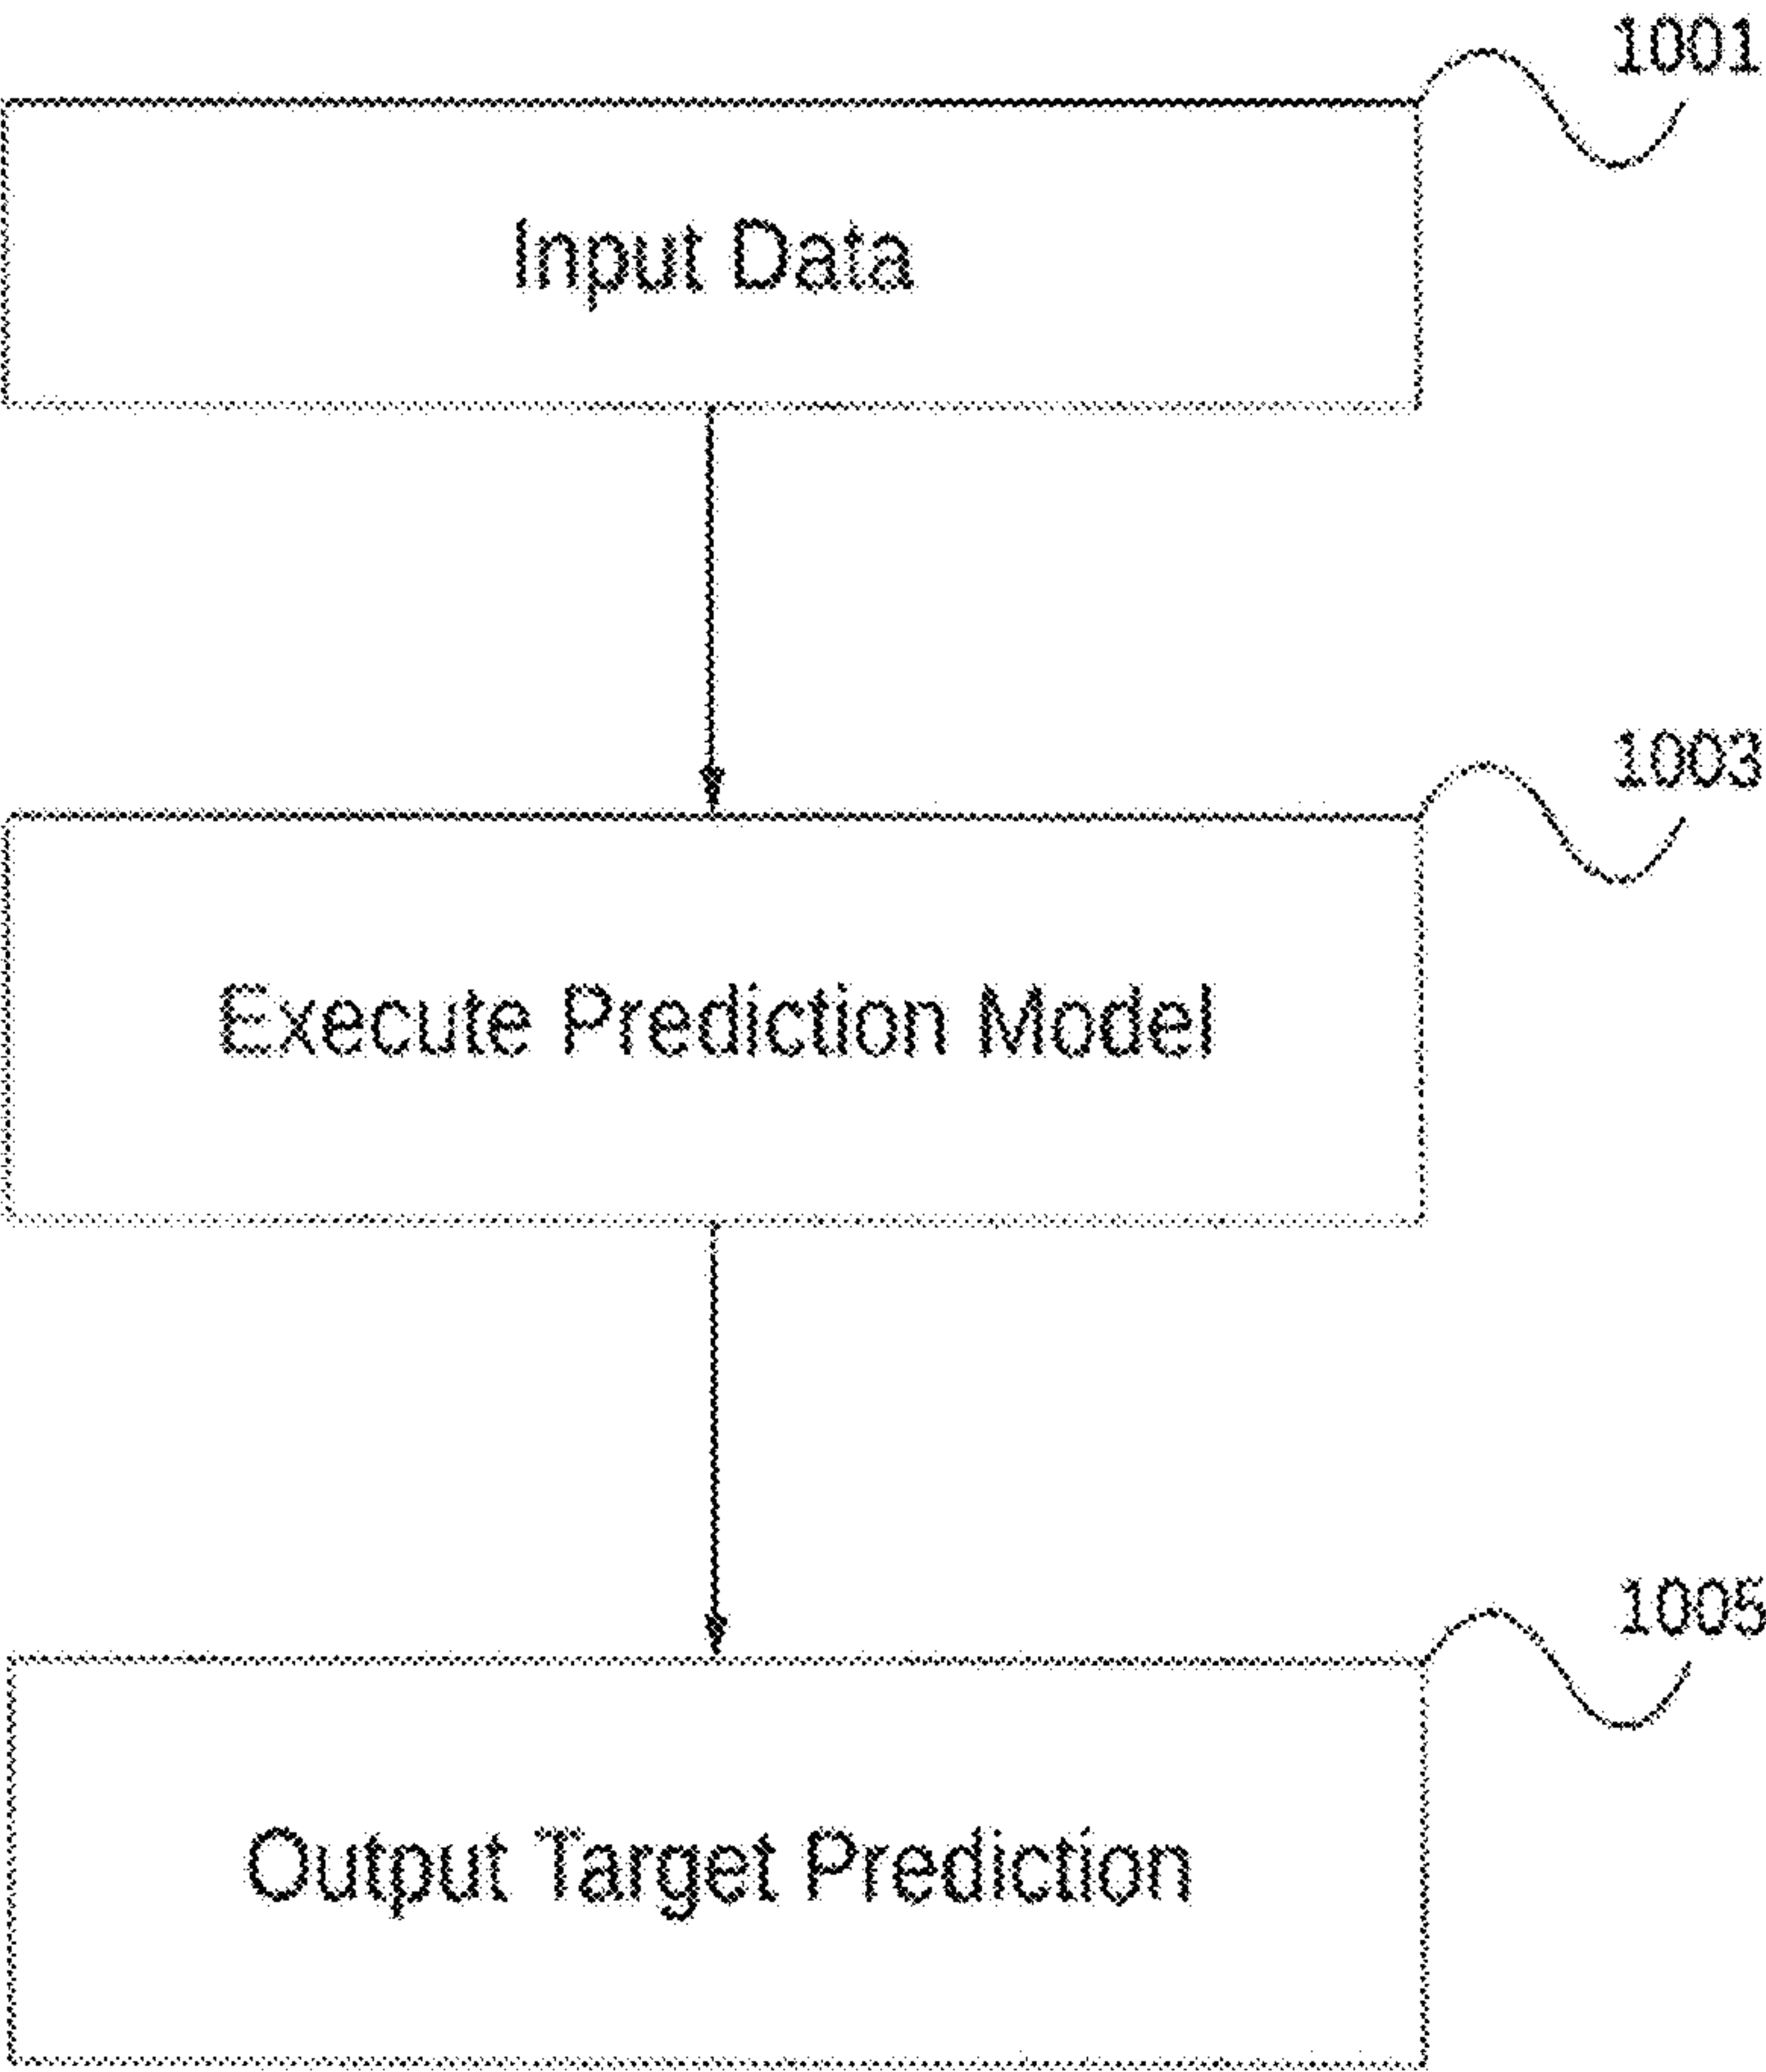


FIG. 10

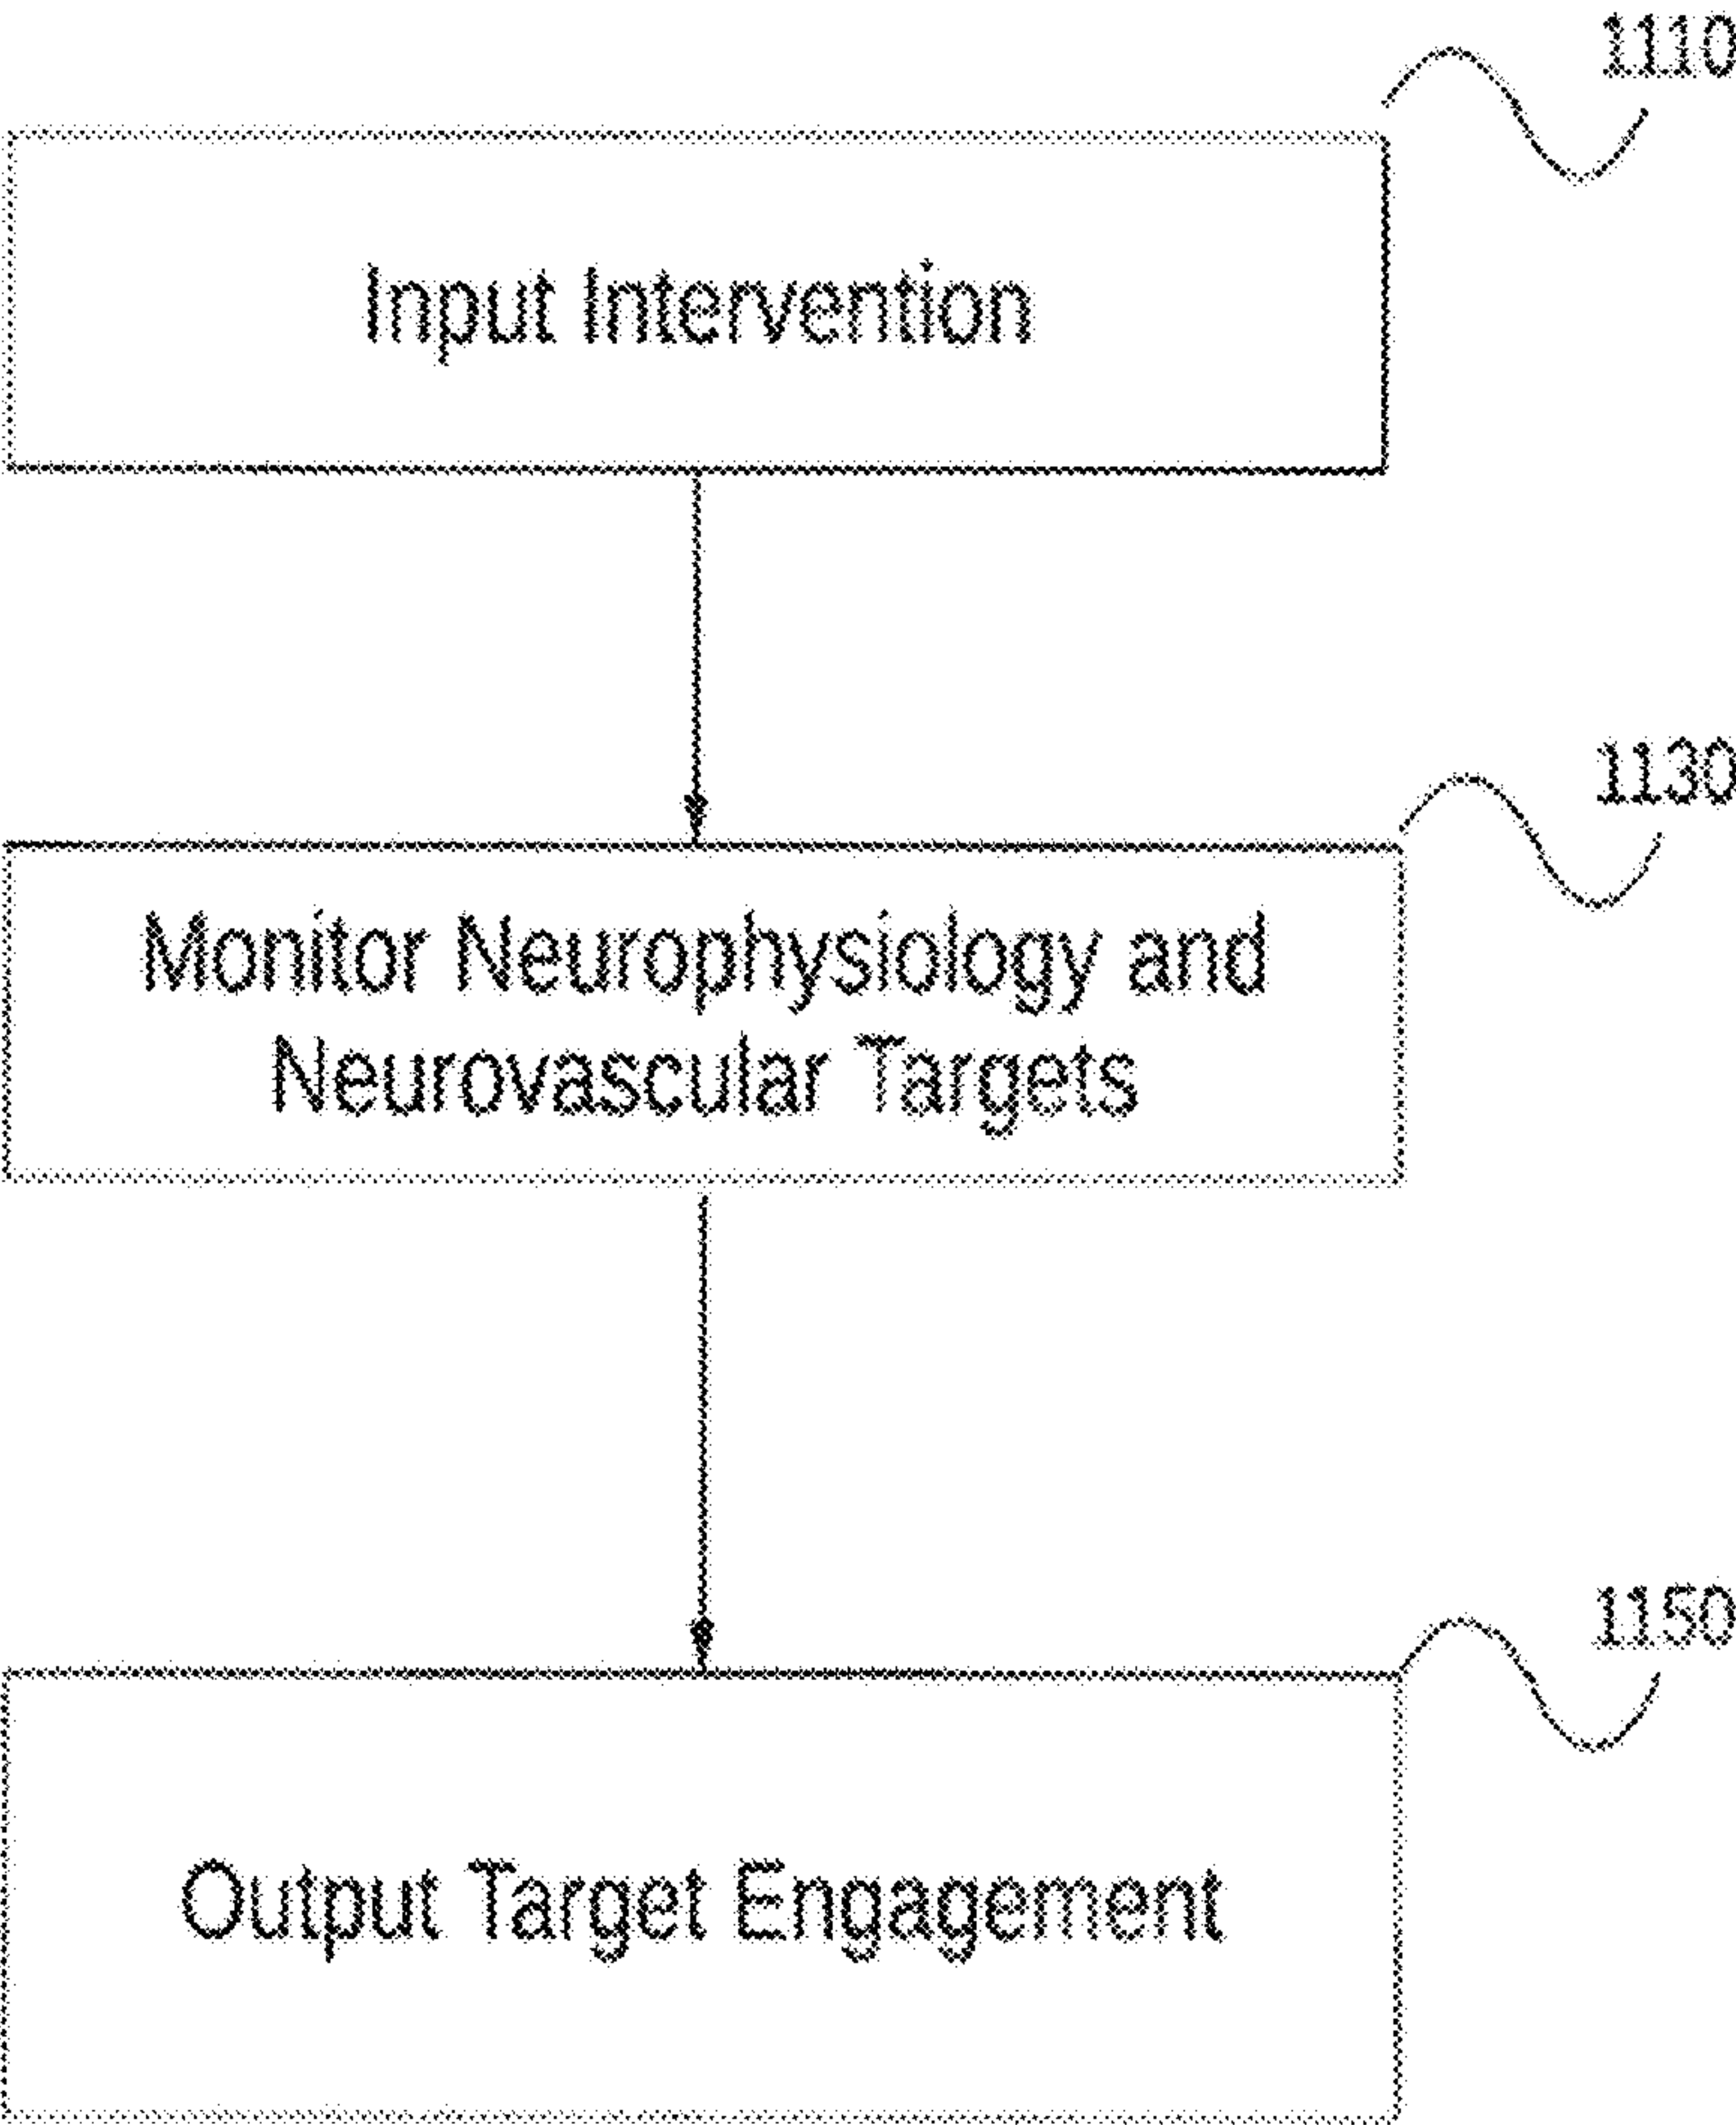


FIG. 11A



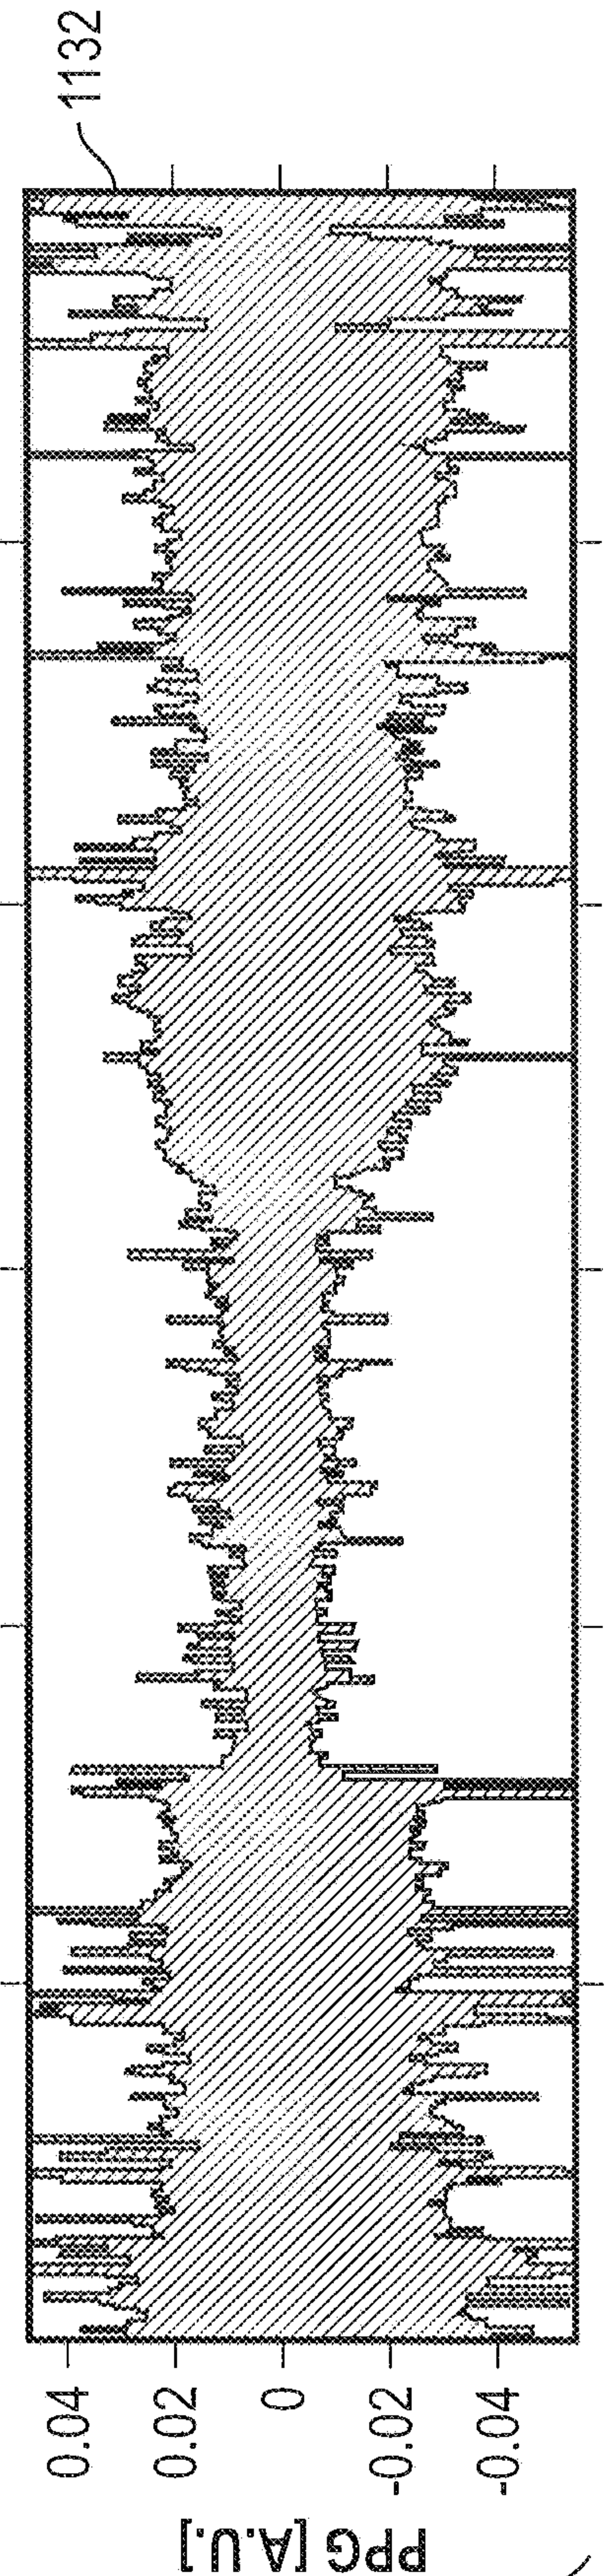


FIG. 11B

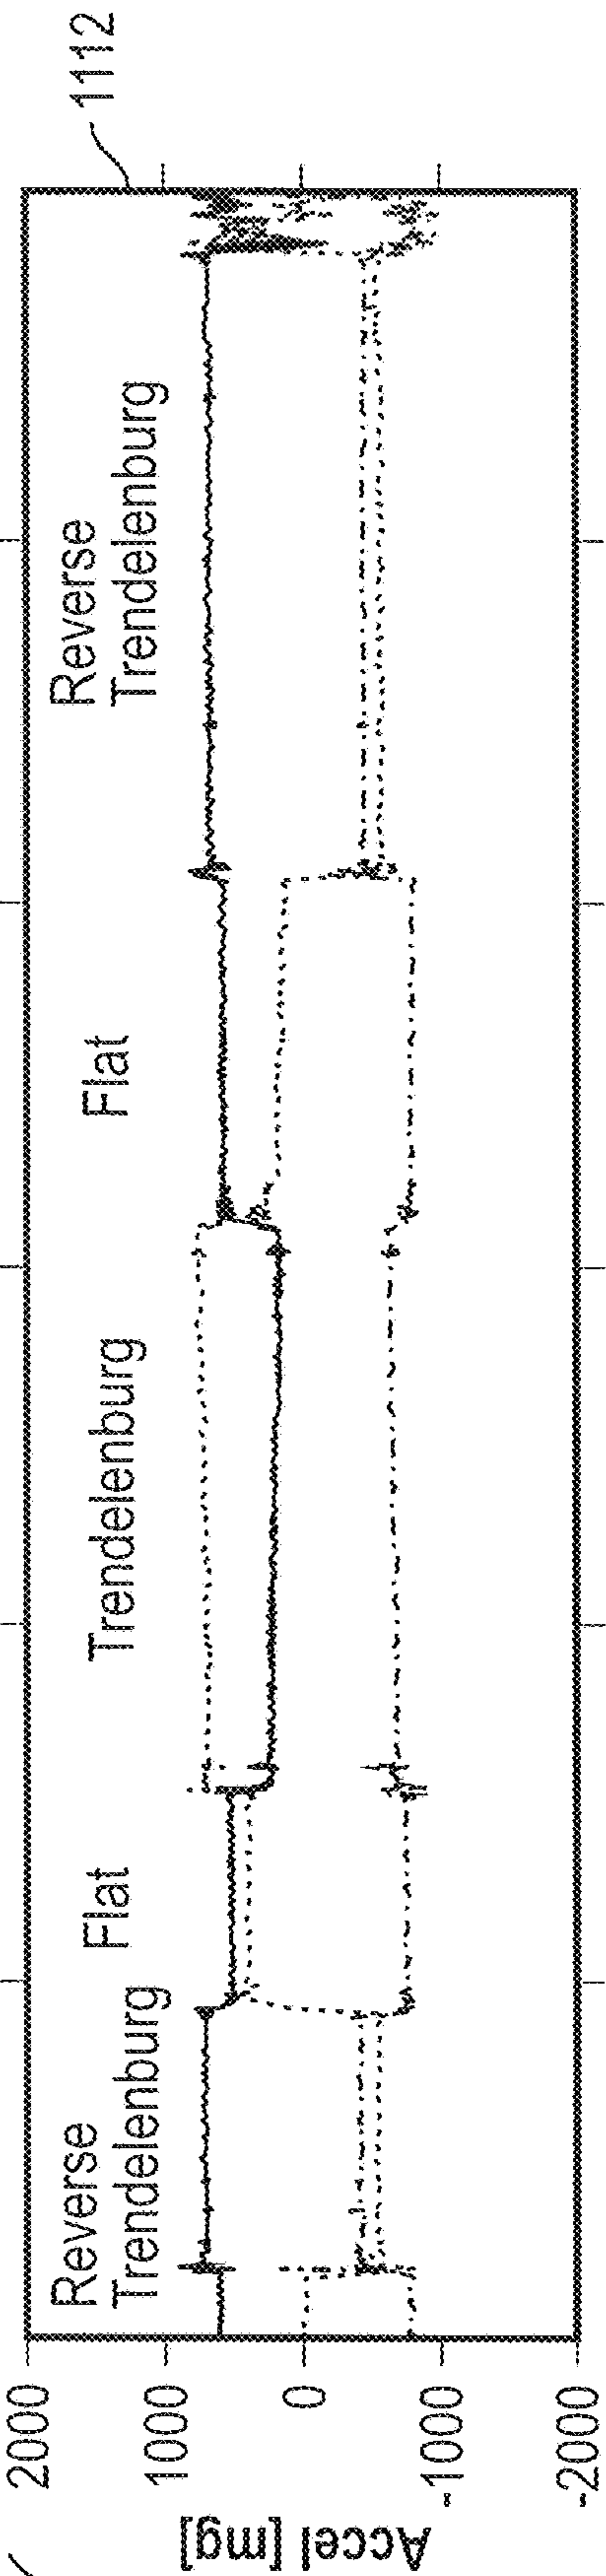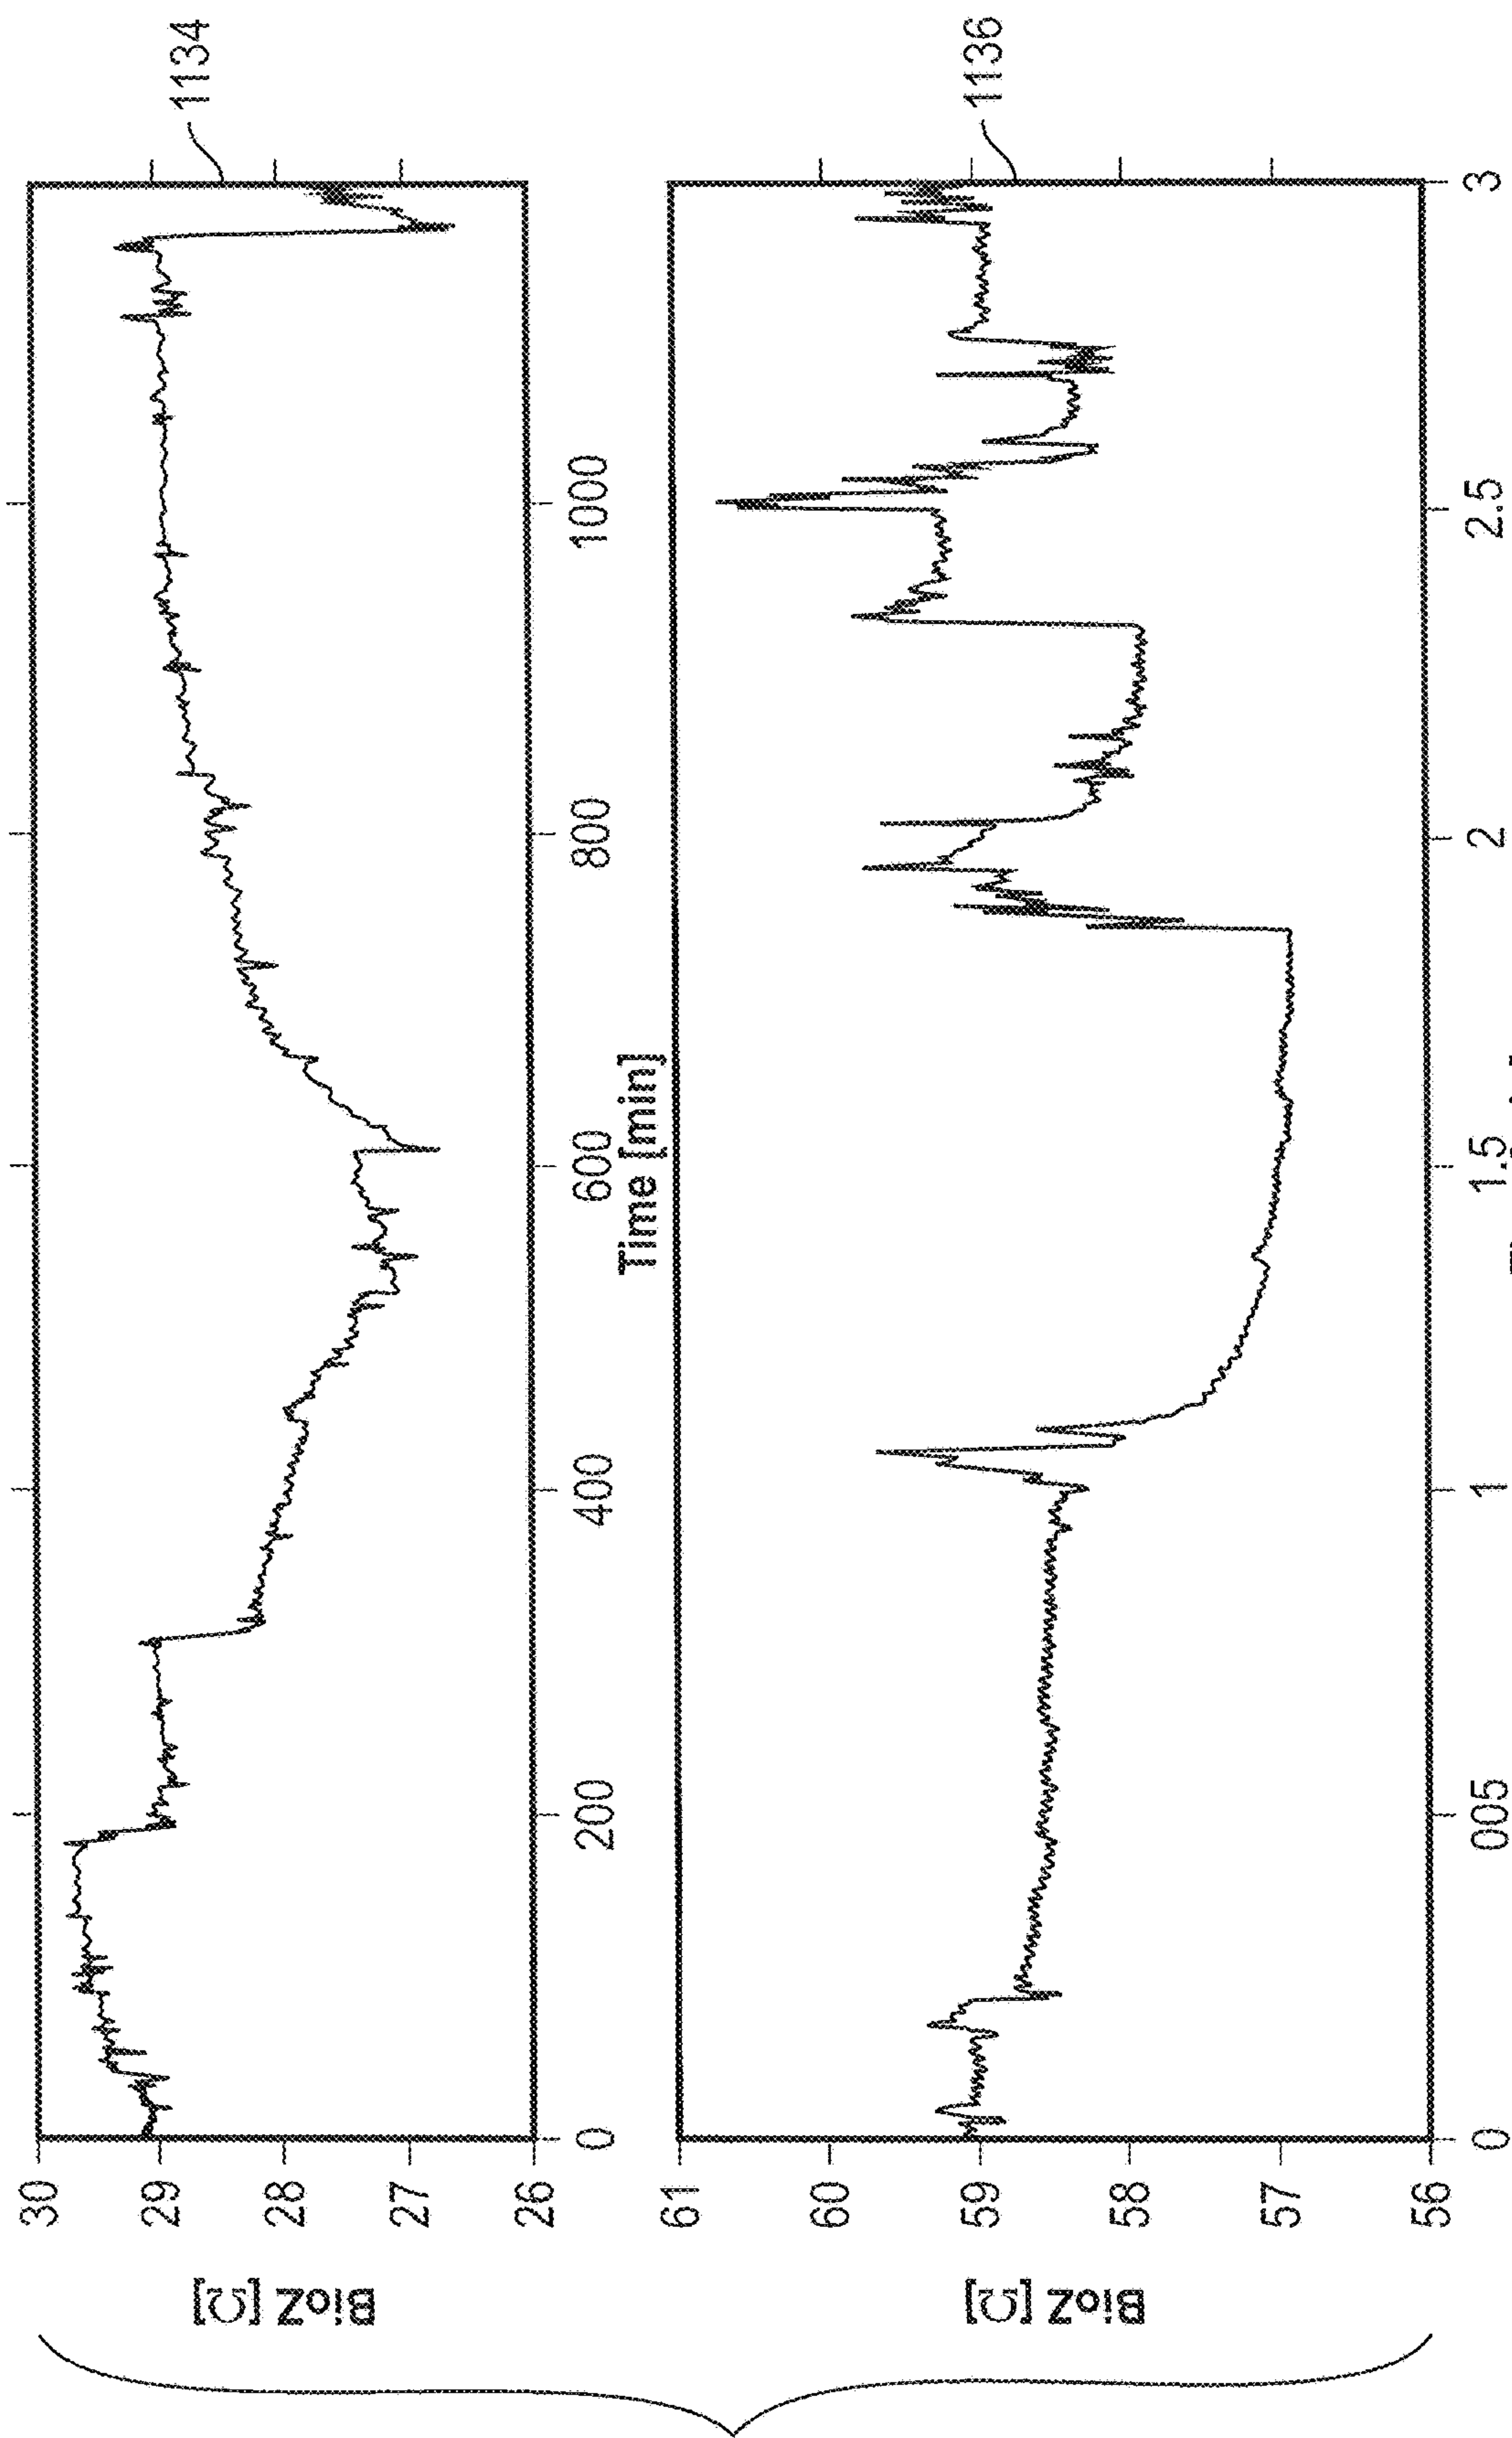

Time [min]
FIG. 11B
(Continued)

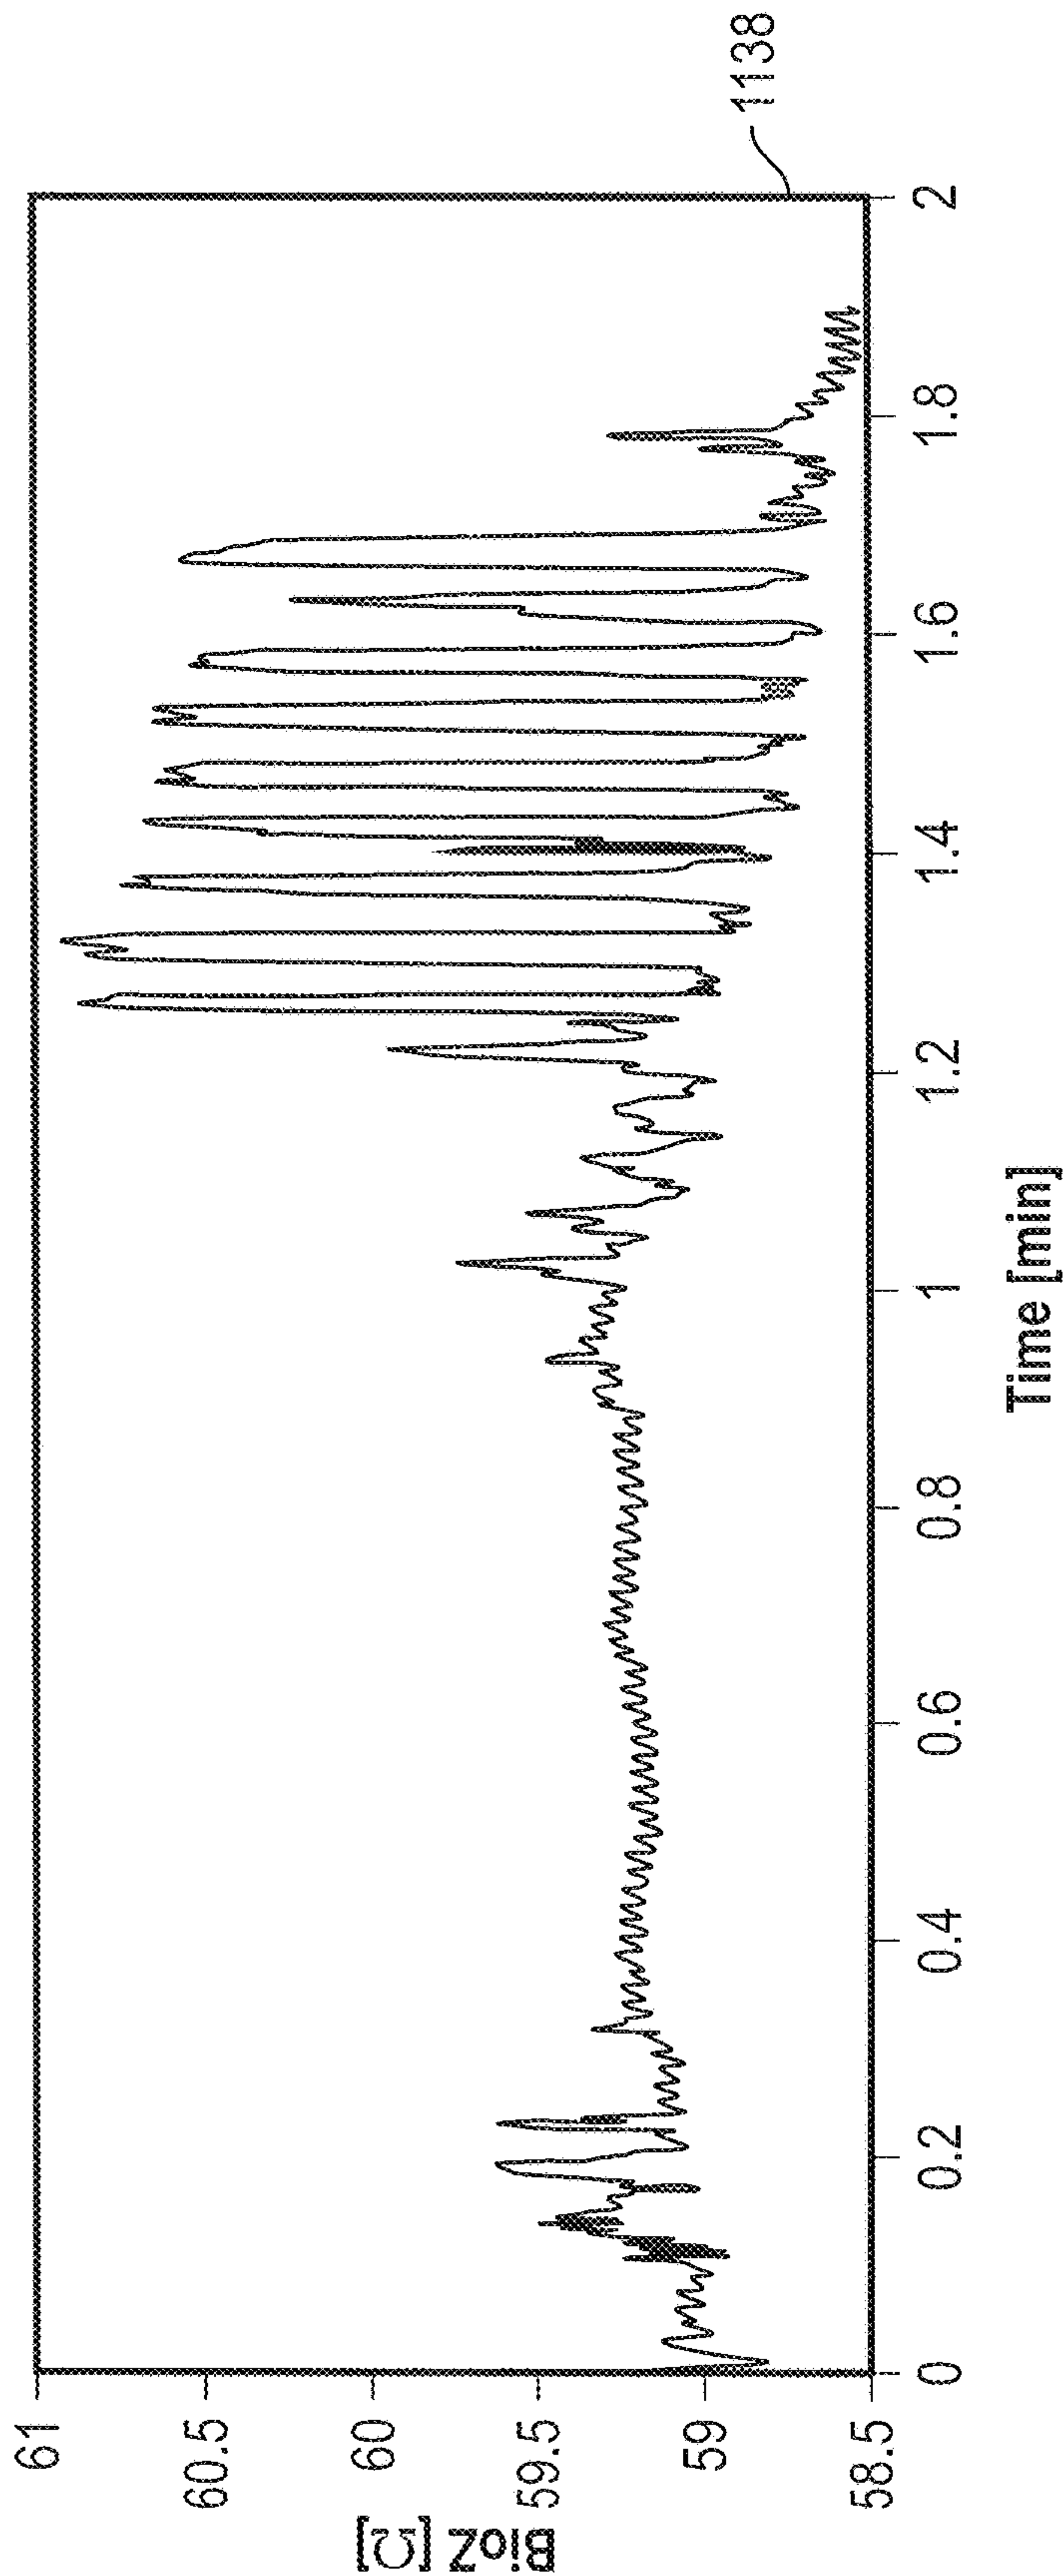


FIG. 11B
(Continued)

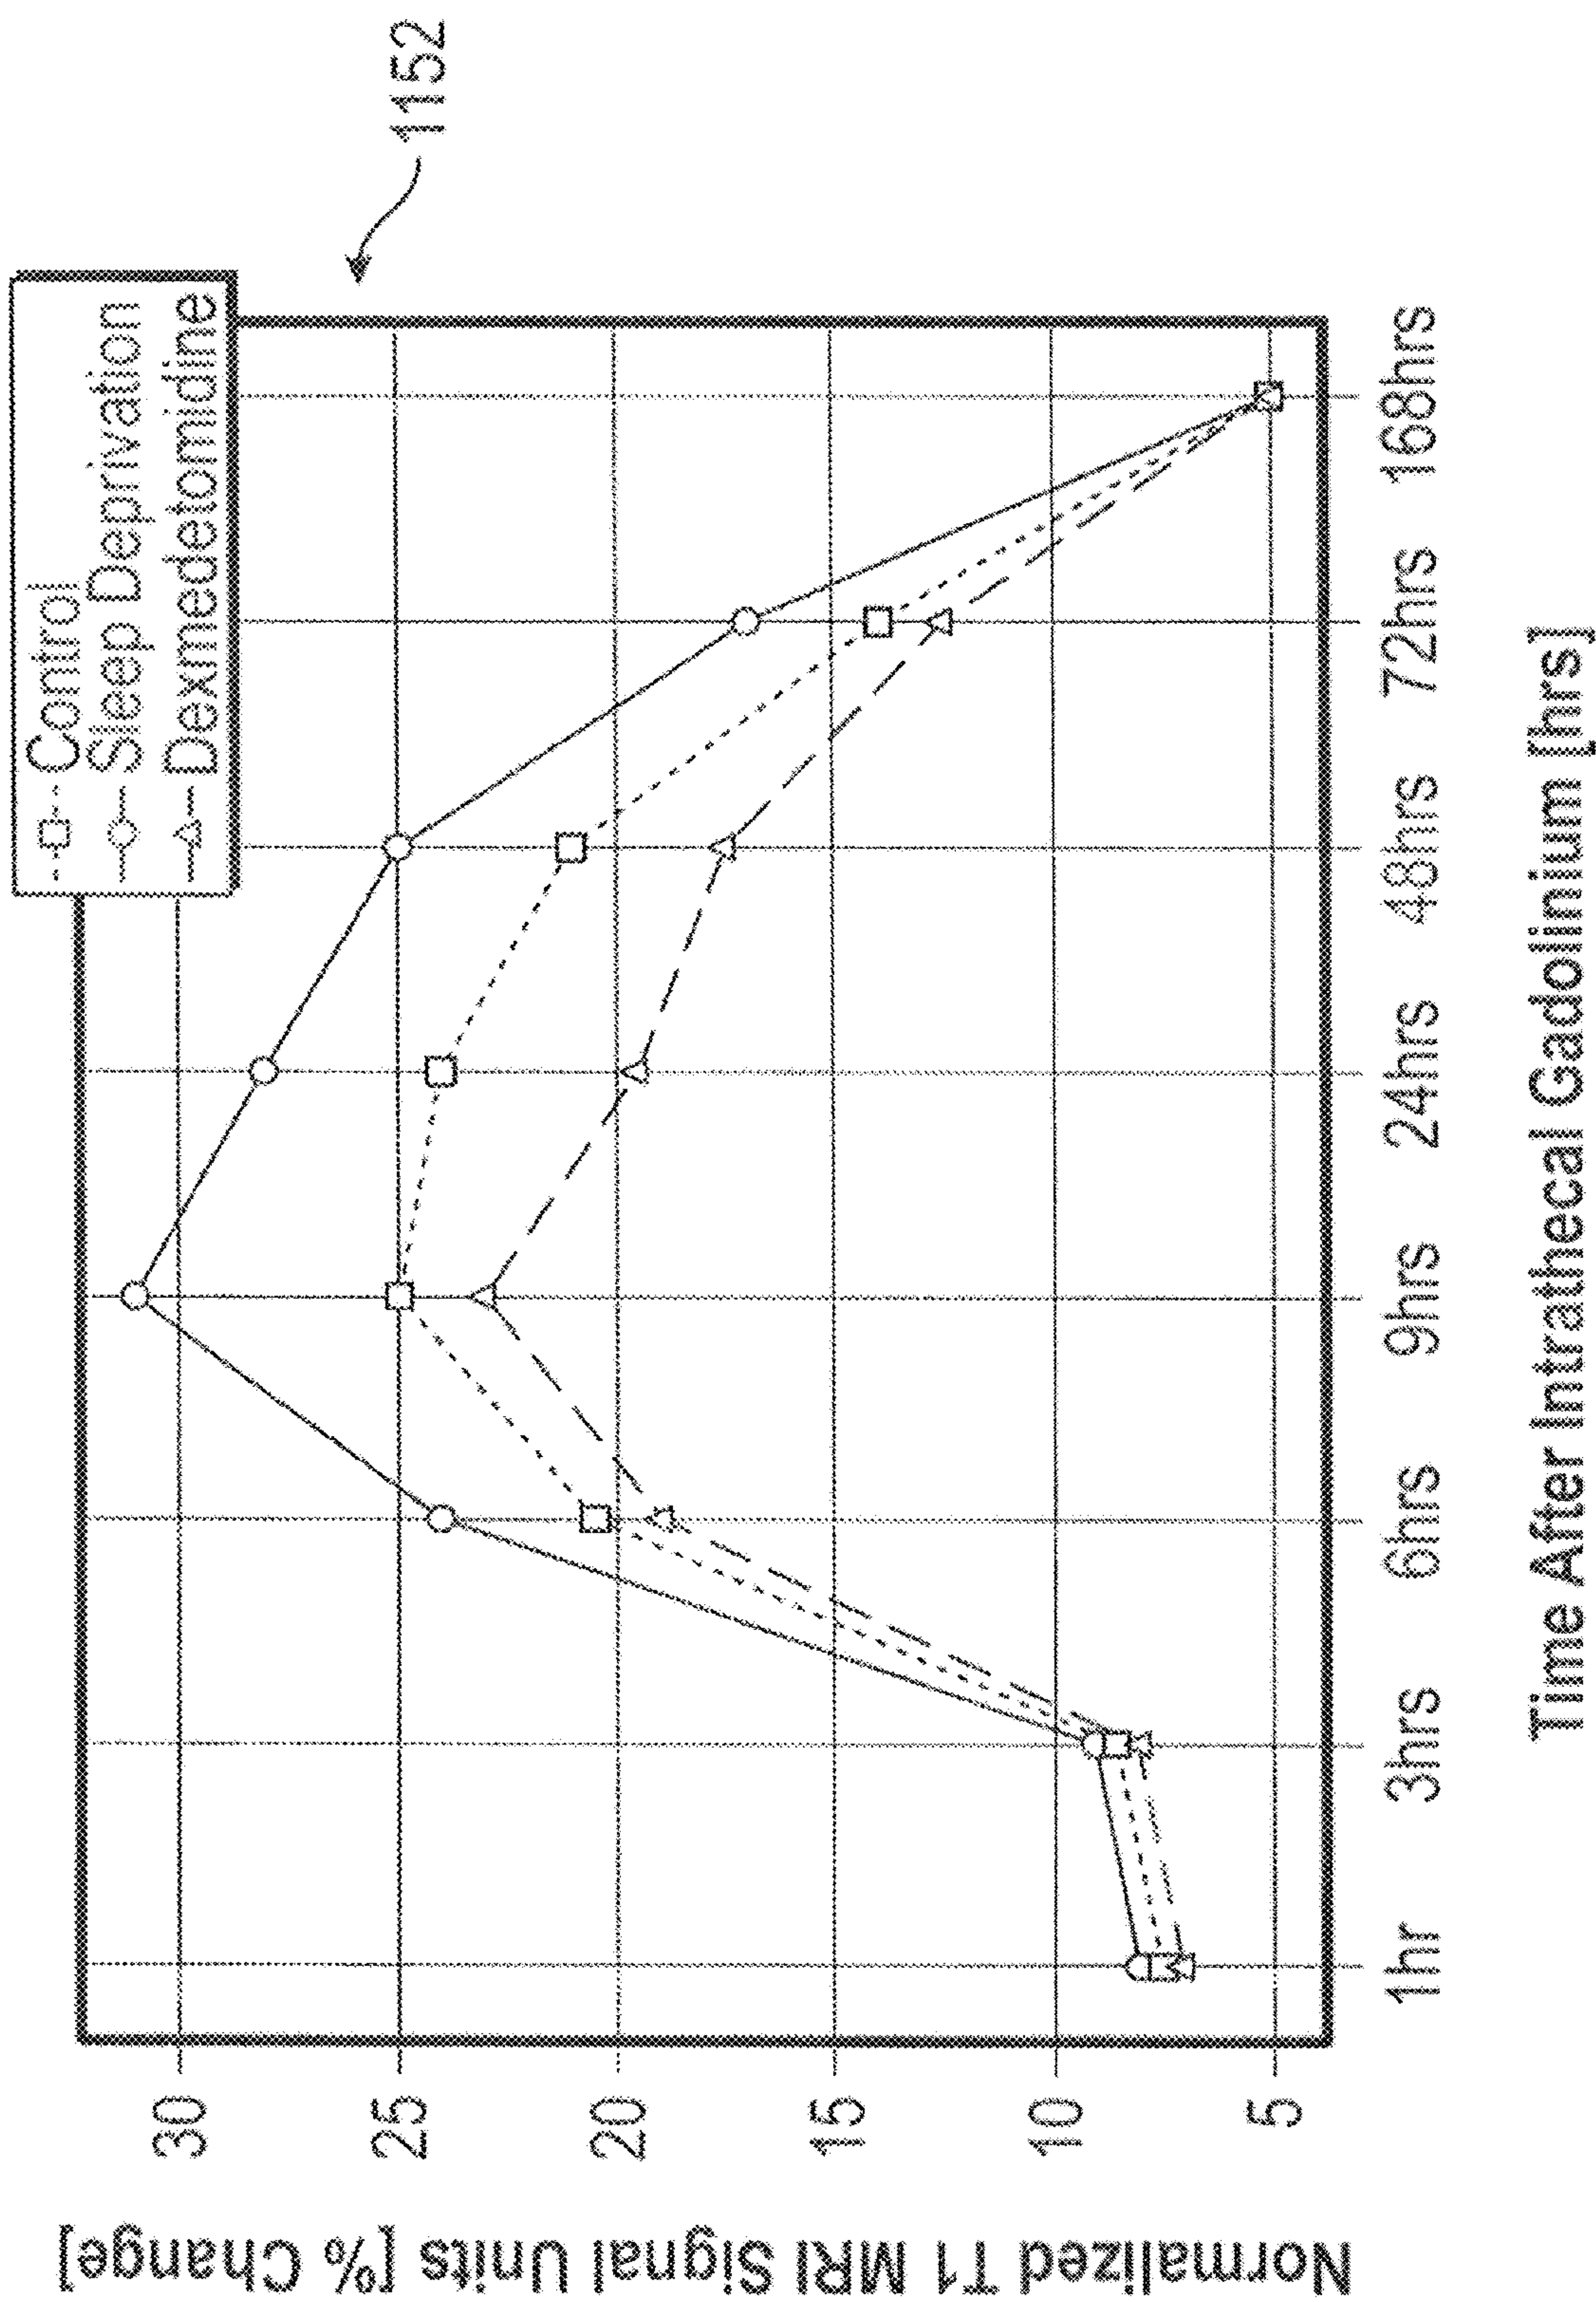


FIG. 11C

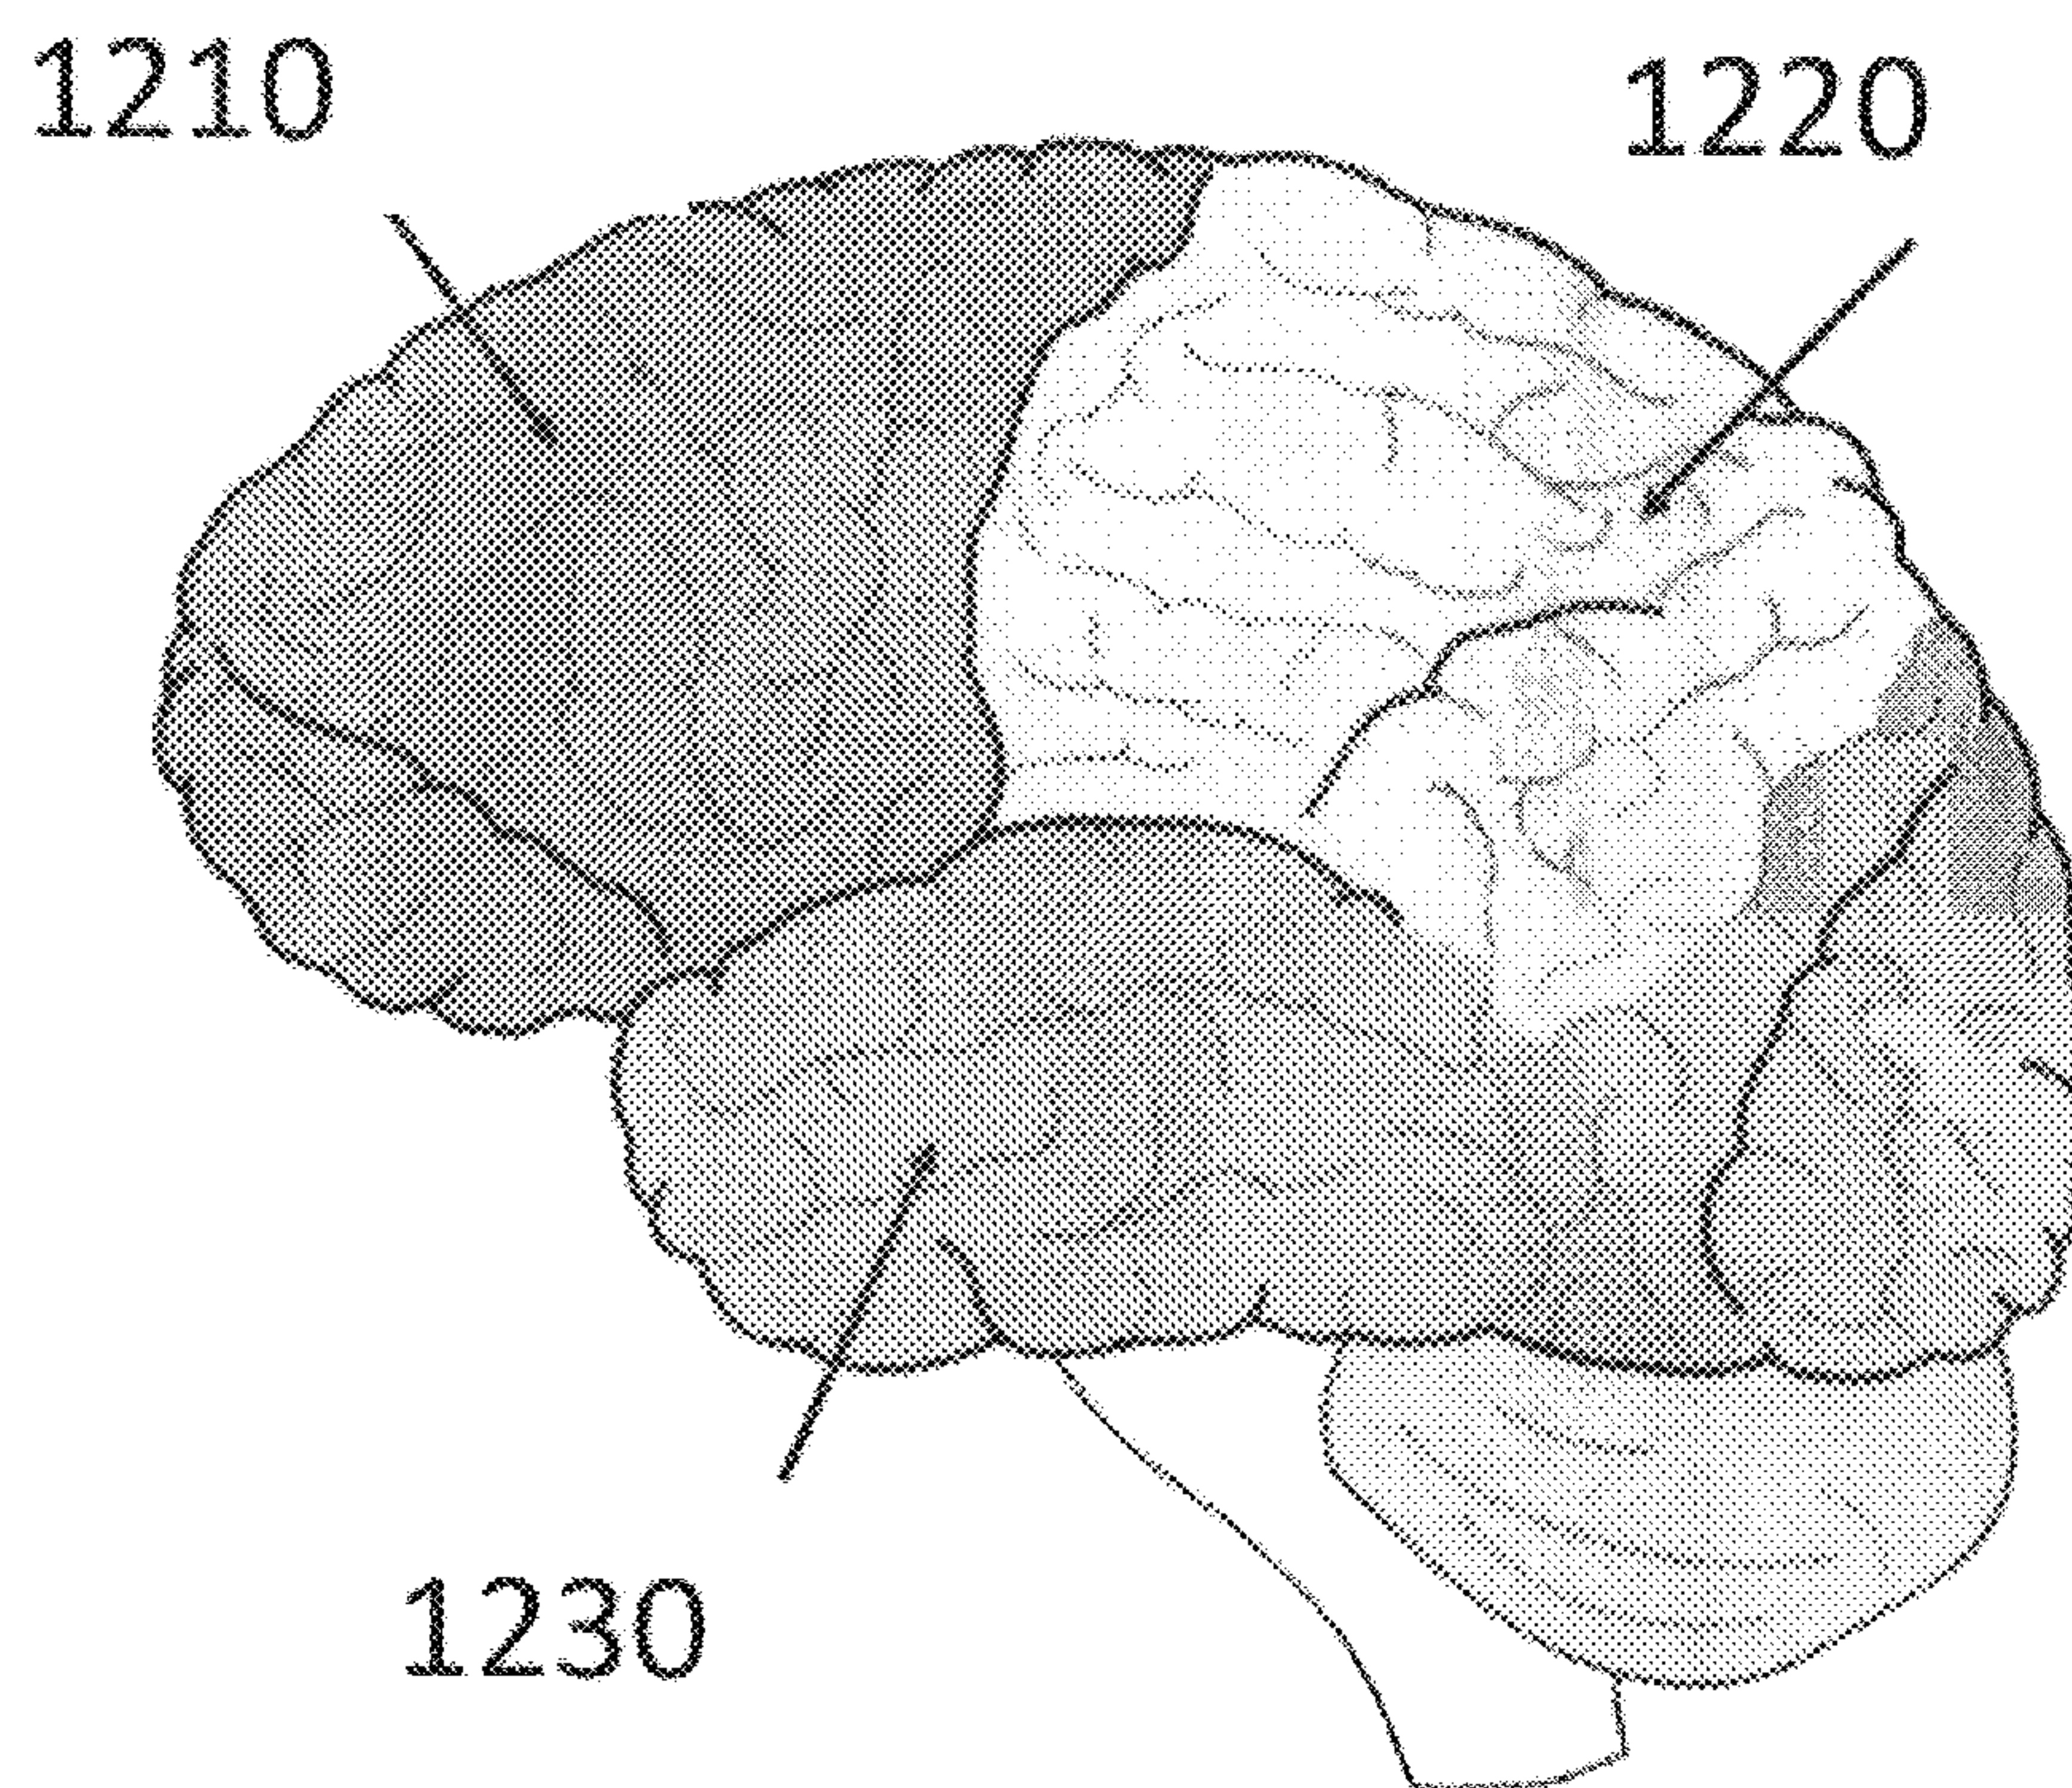


FIG. 12A

wearable
device 1250

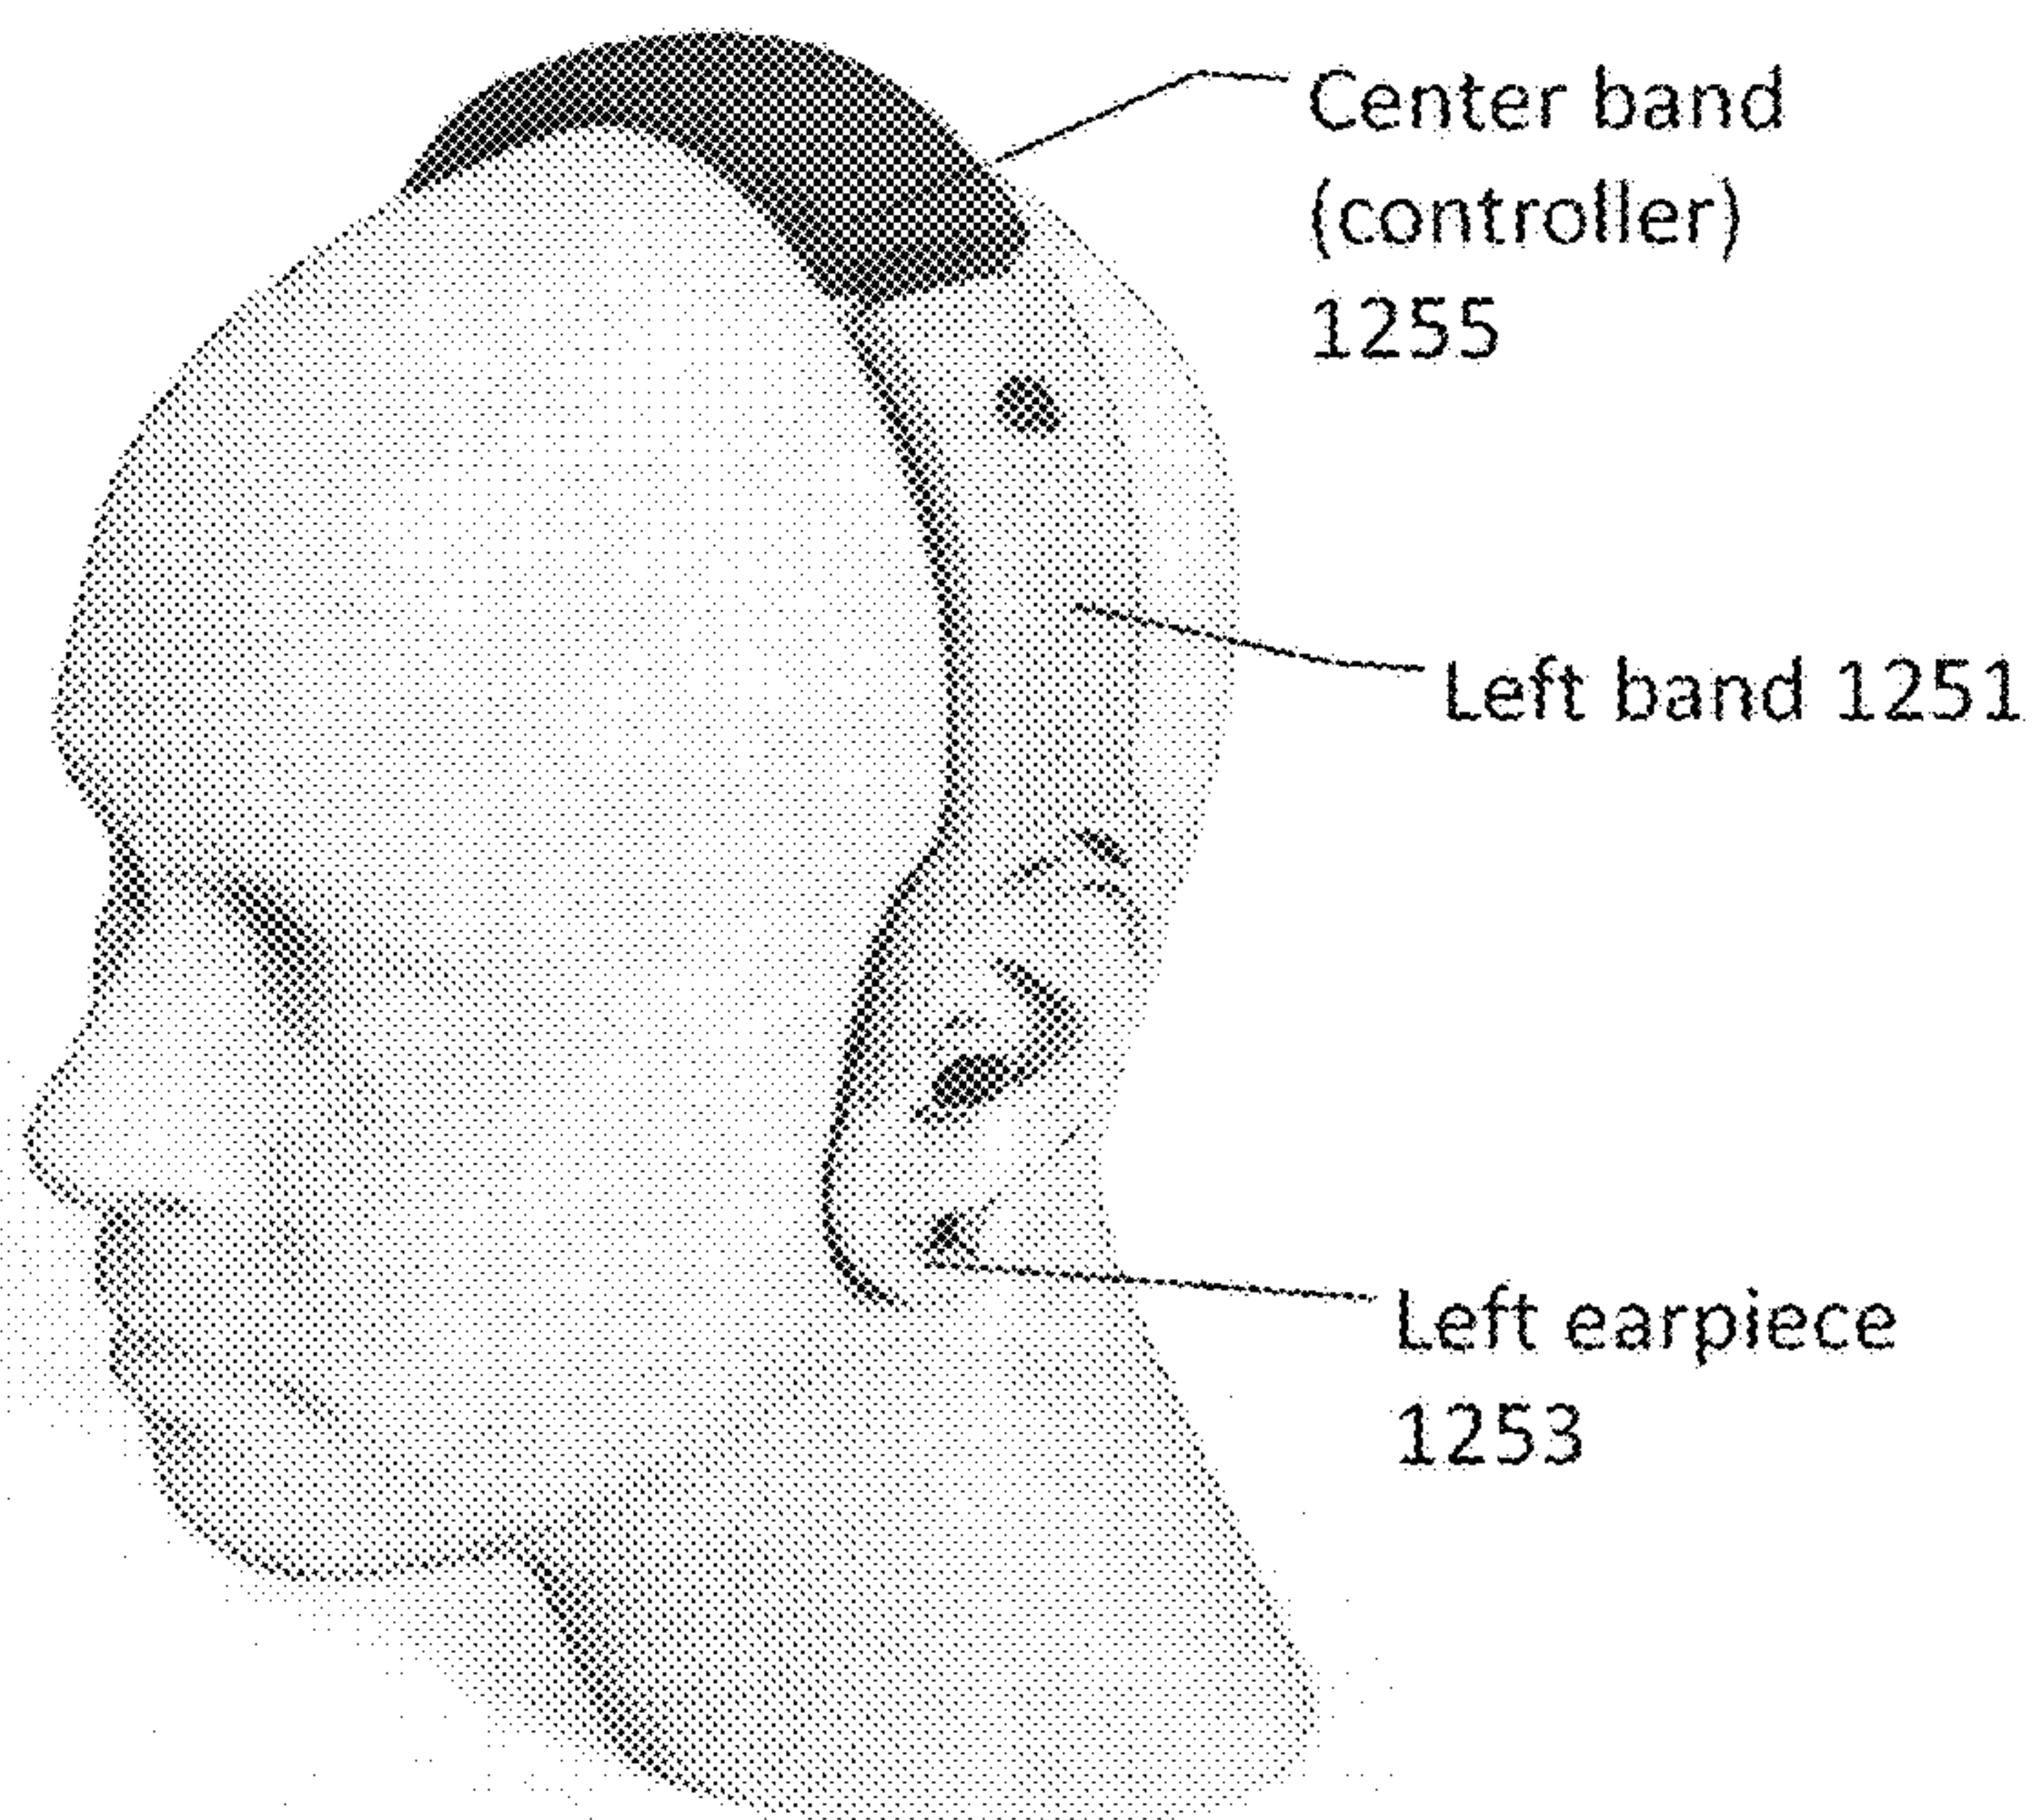


FIG. 12B

wearable
device 1250

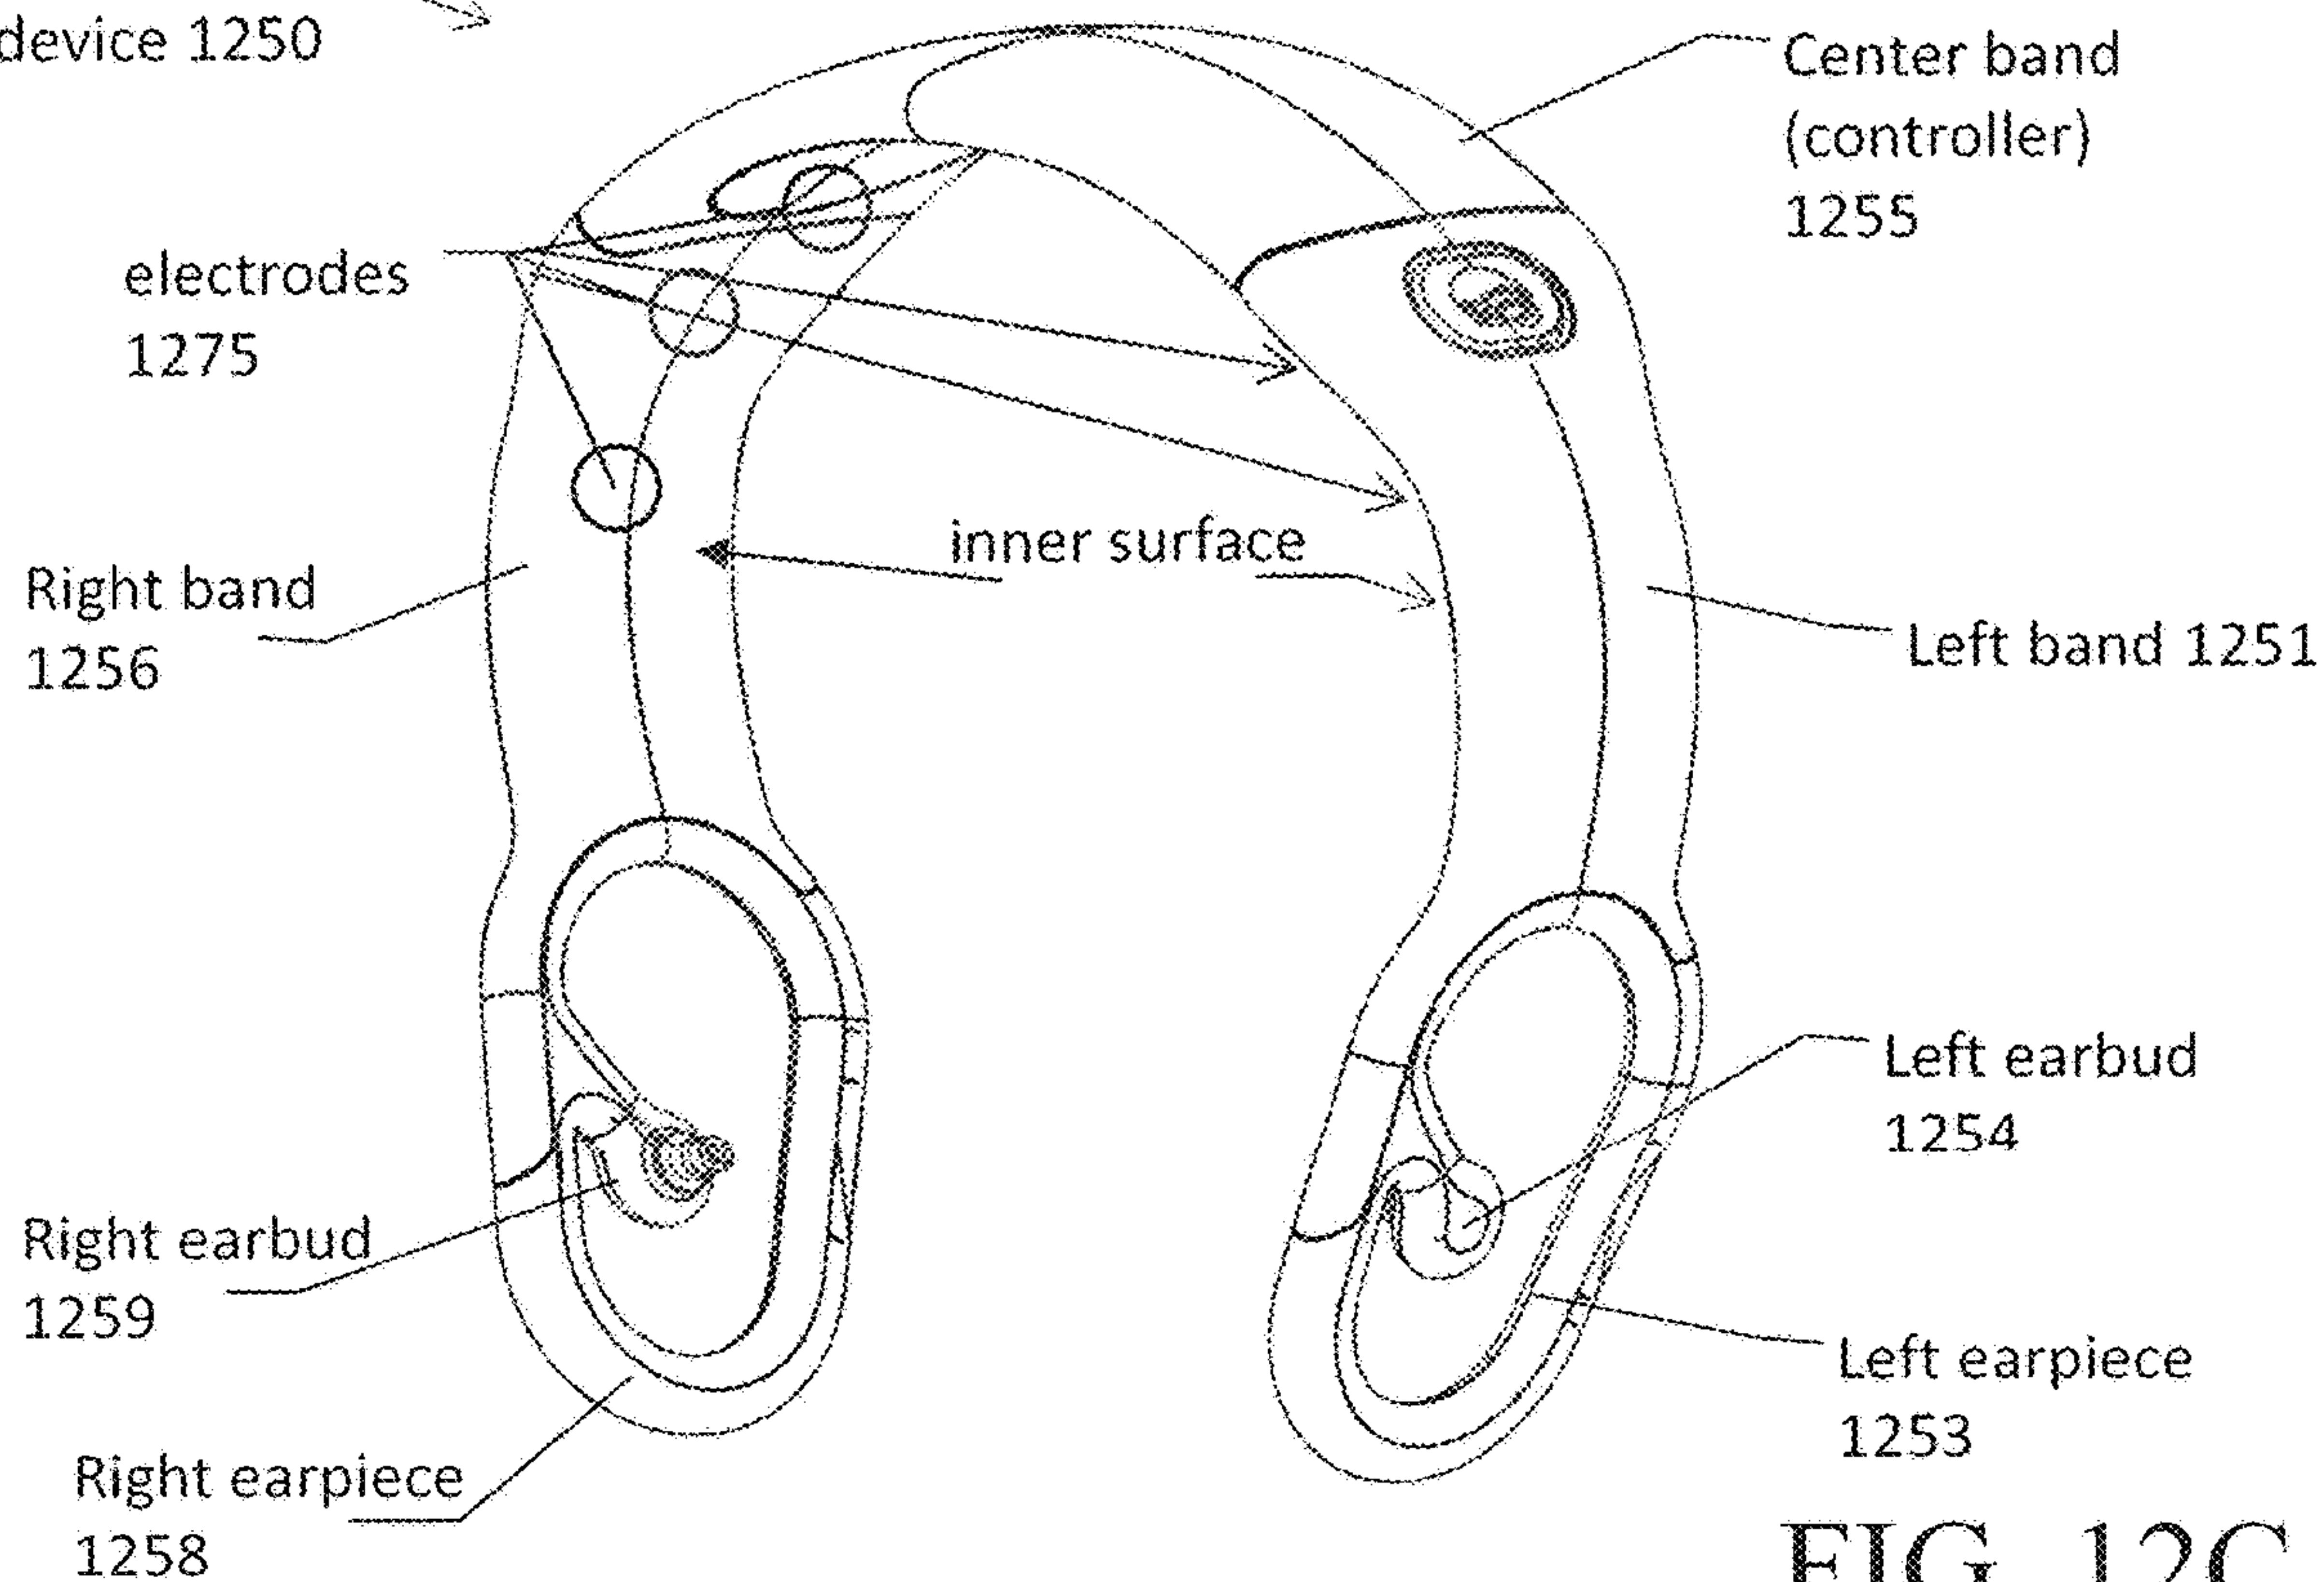


FIG. 12C

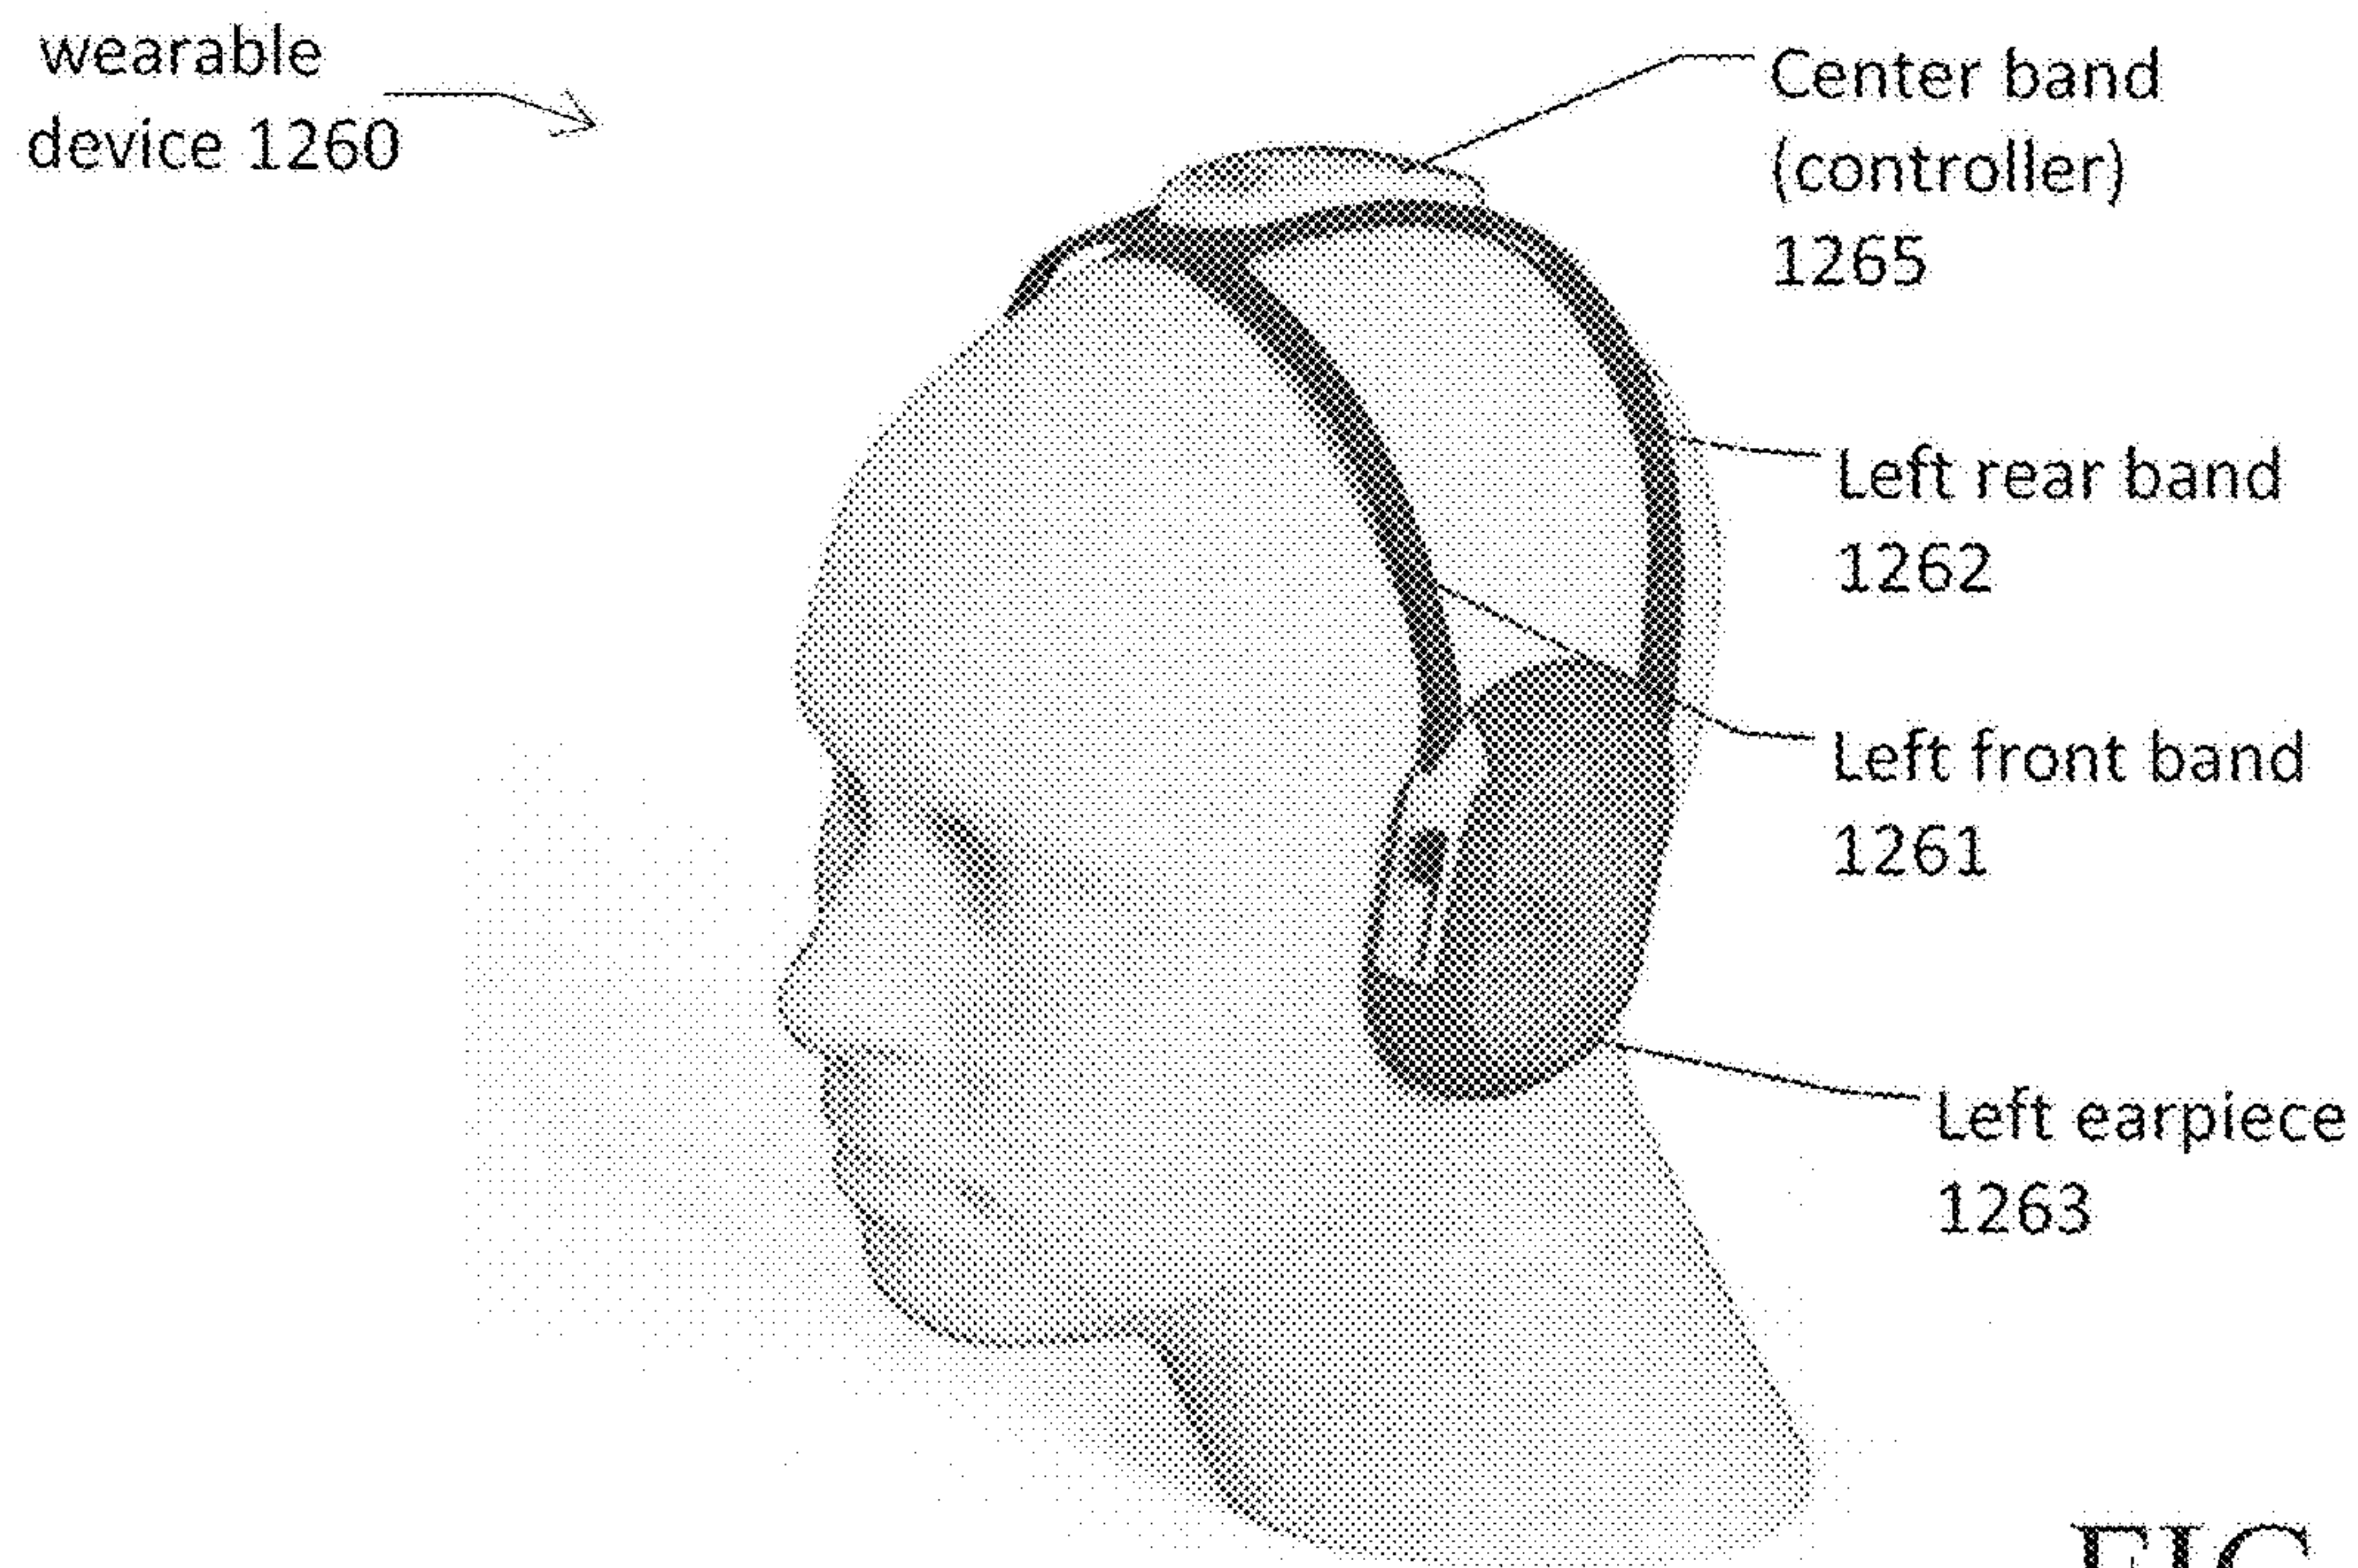


FIG. 12D

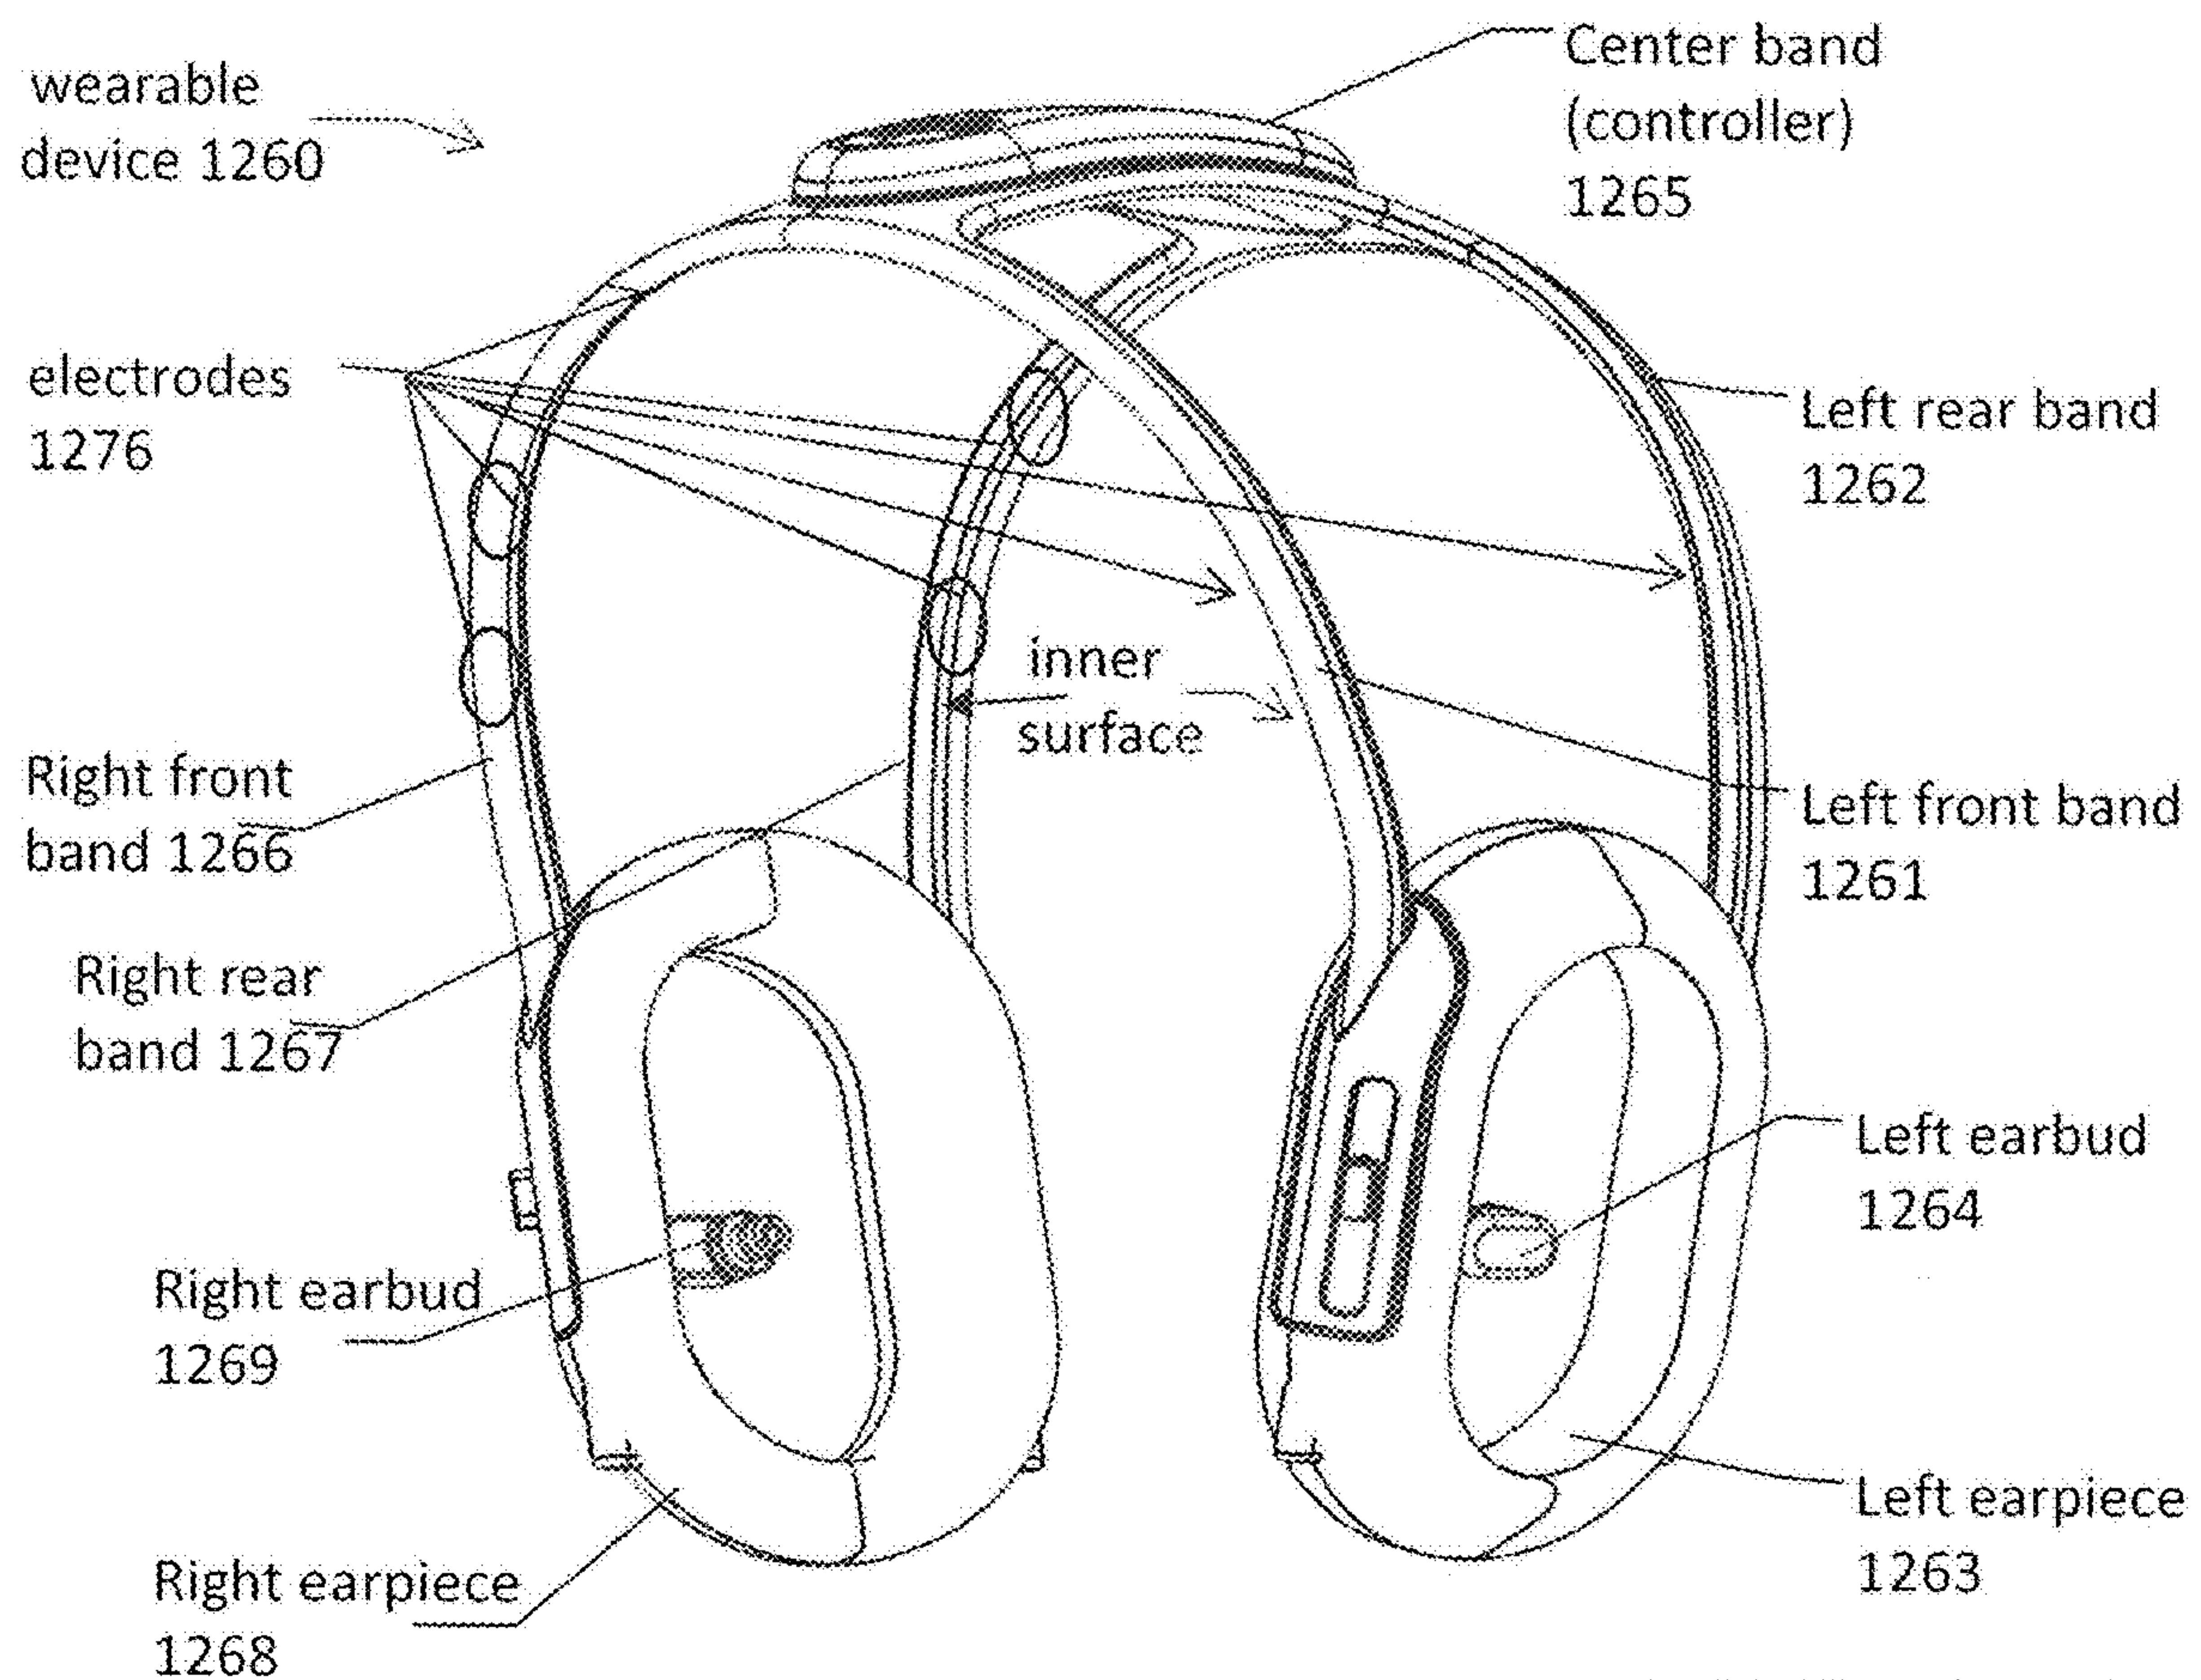
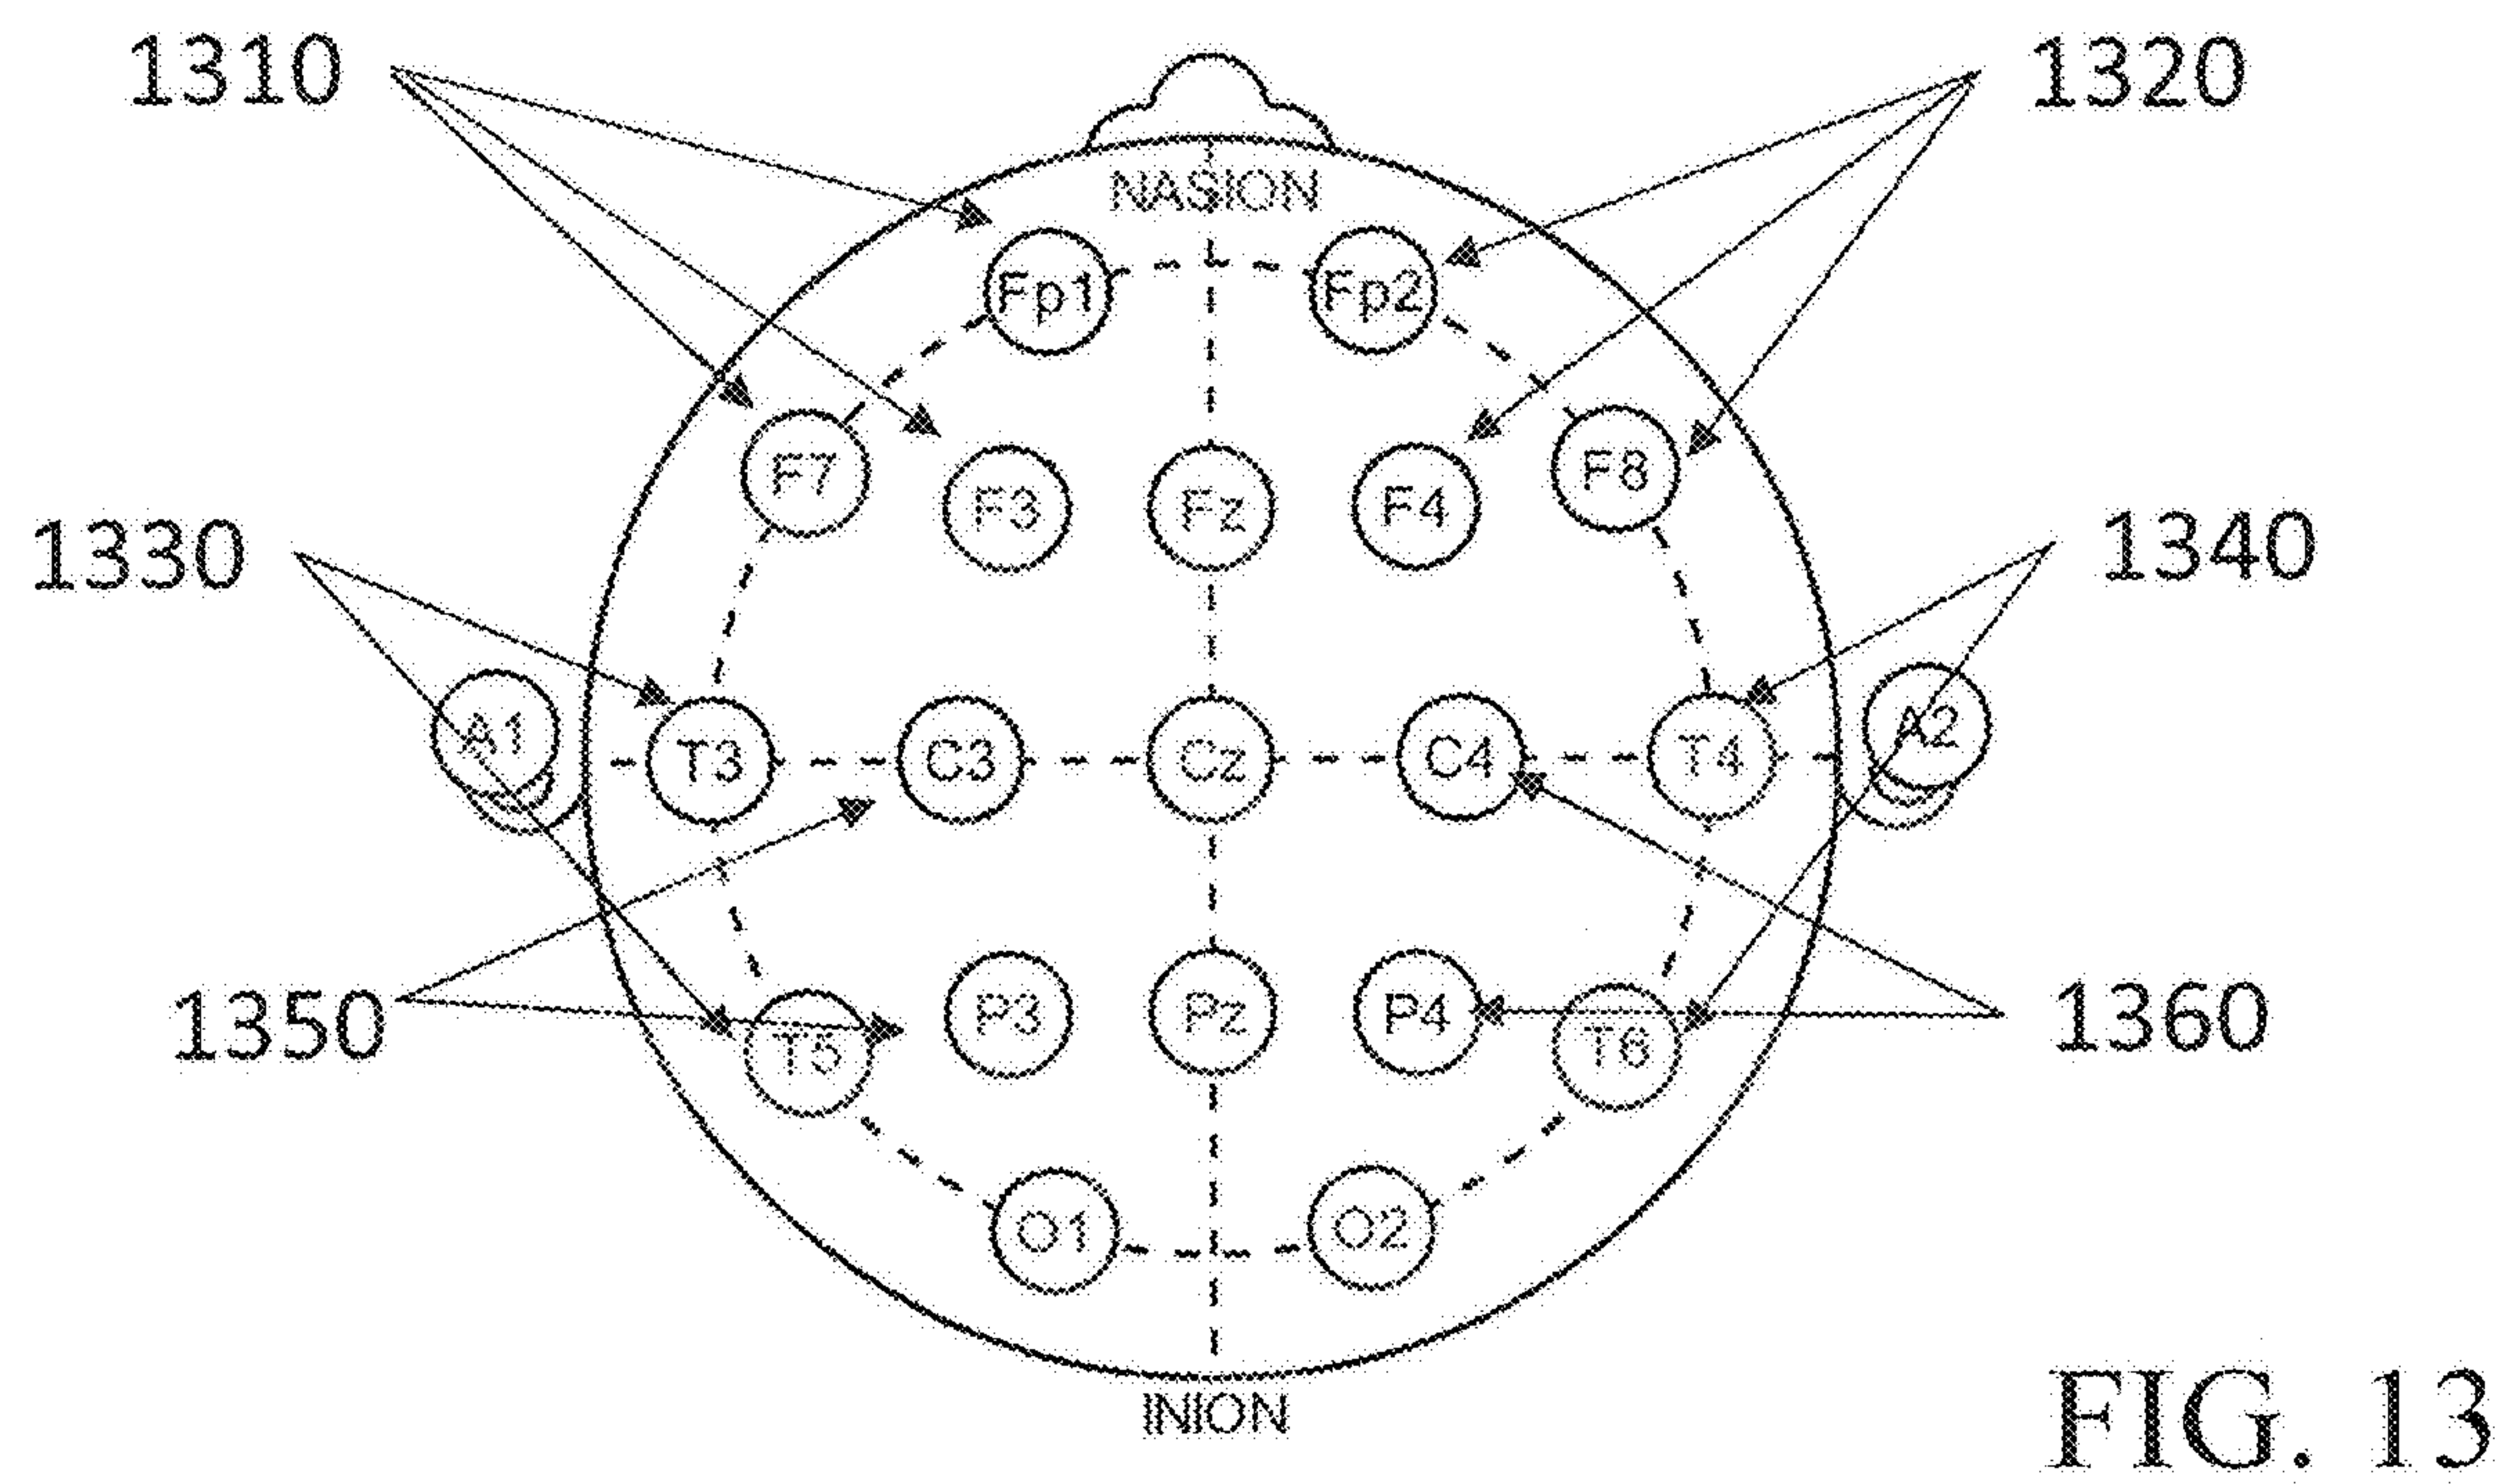


FIG. 12E



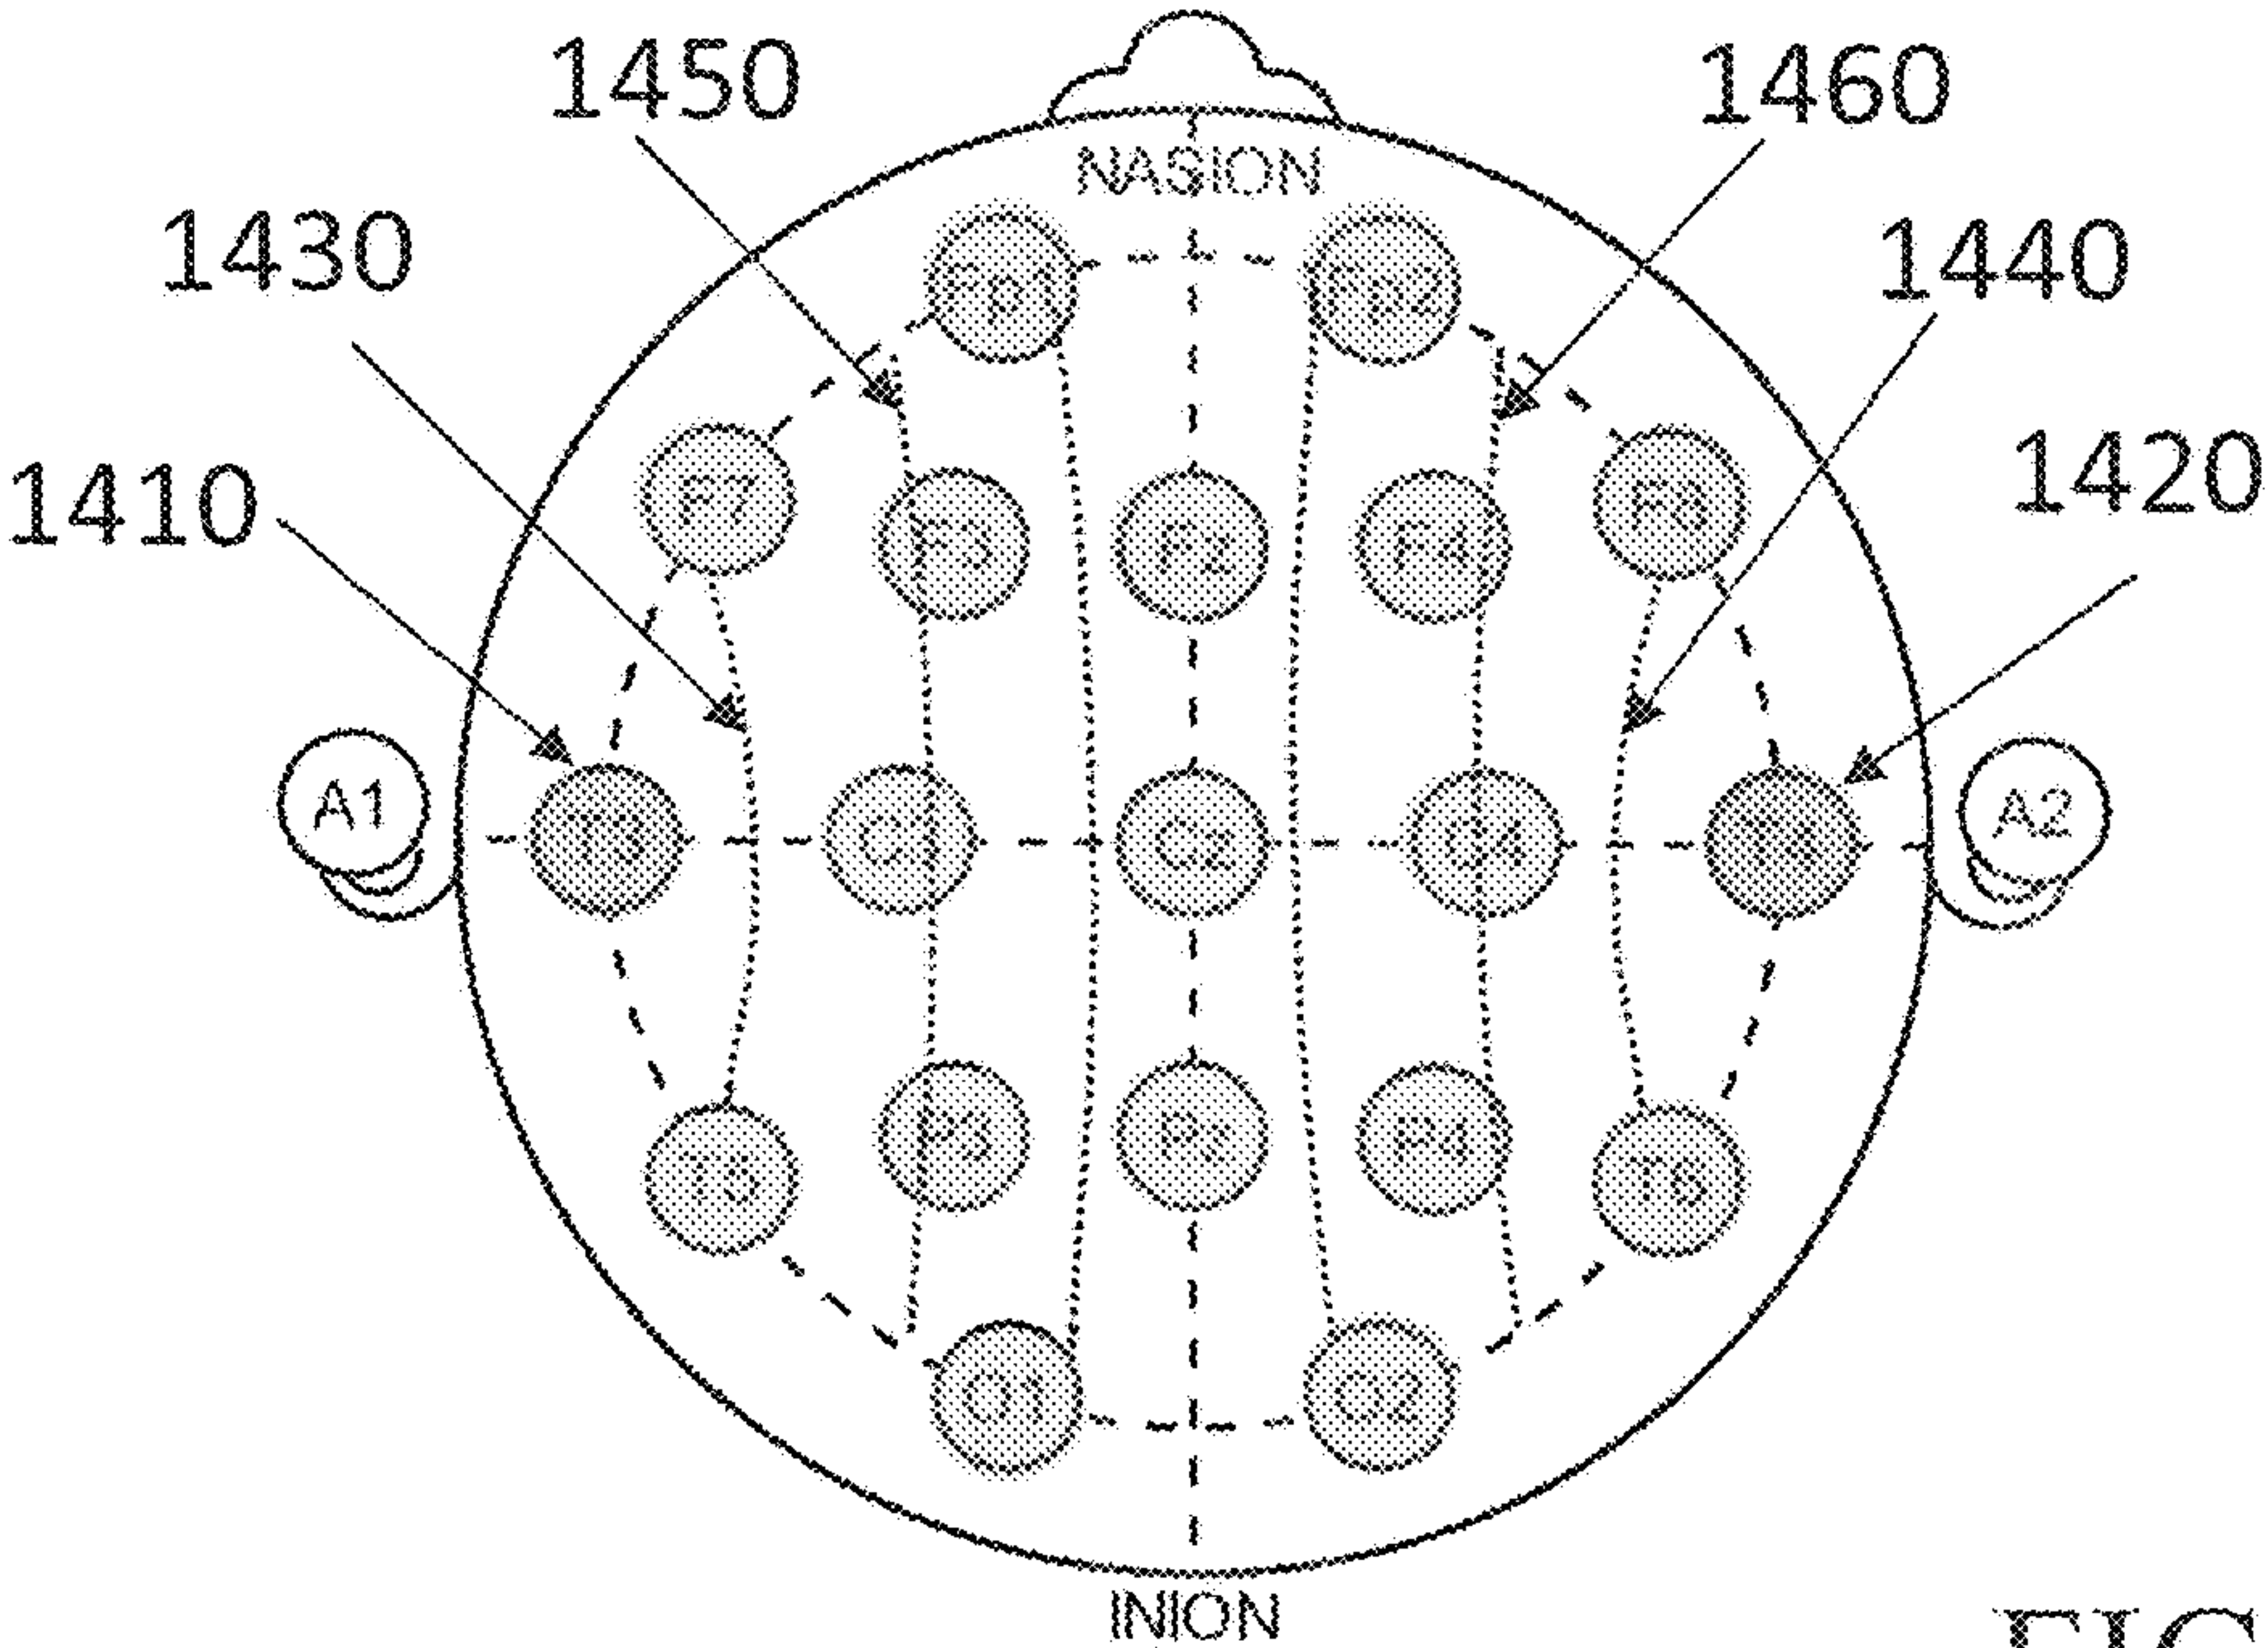


FIG. 14A

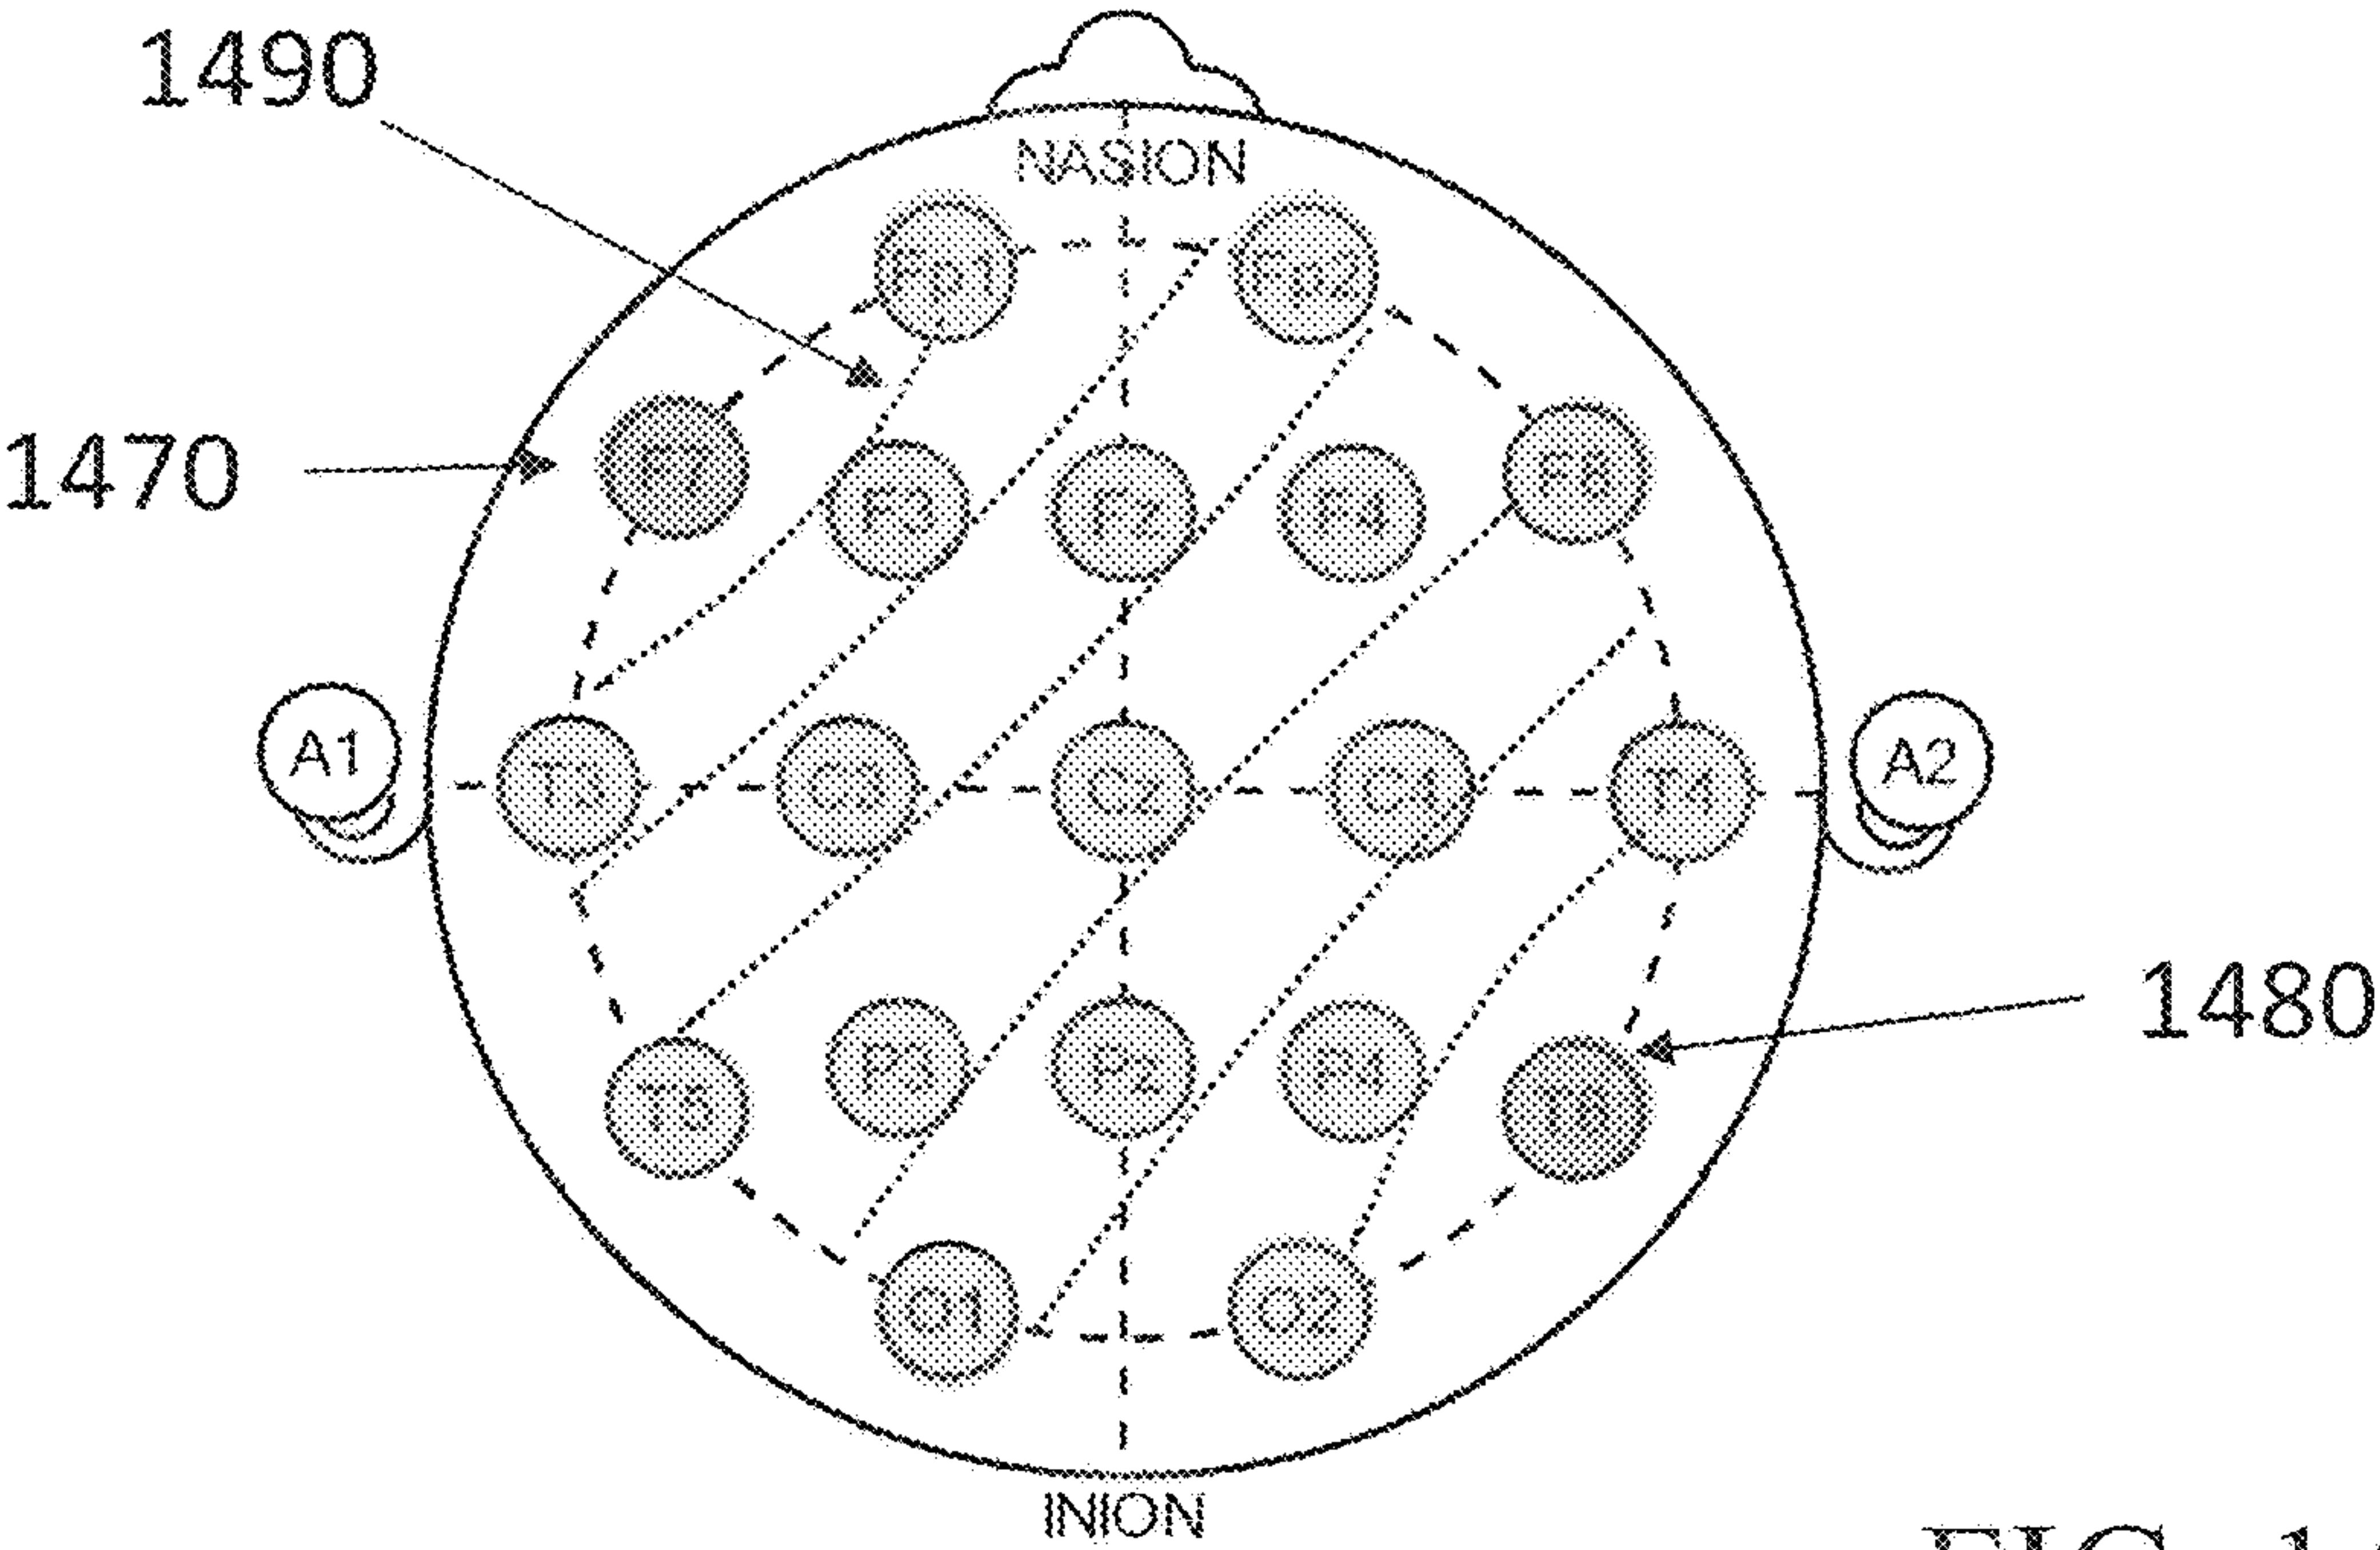
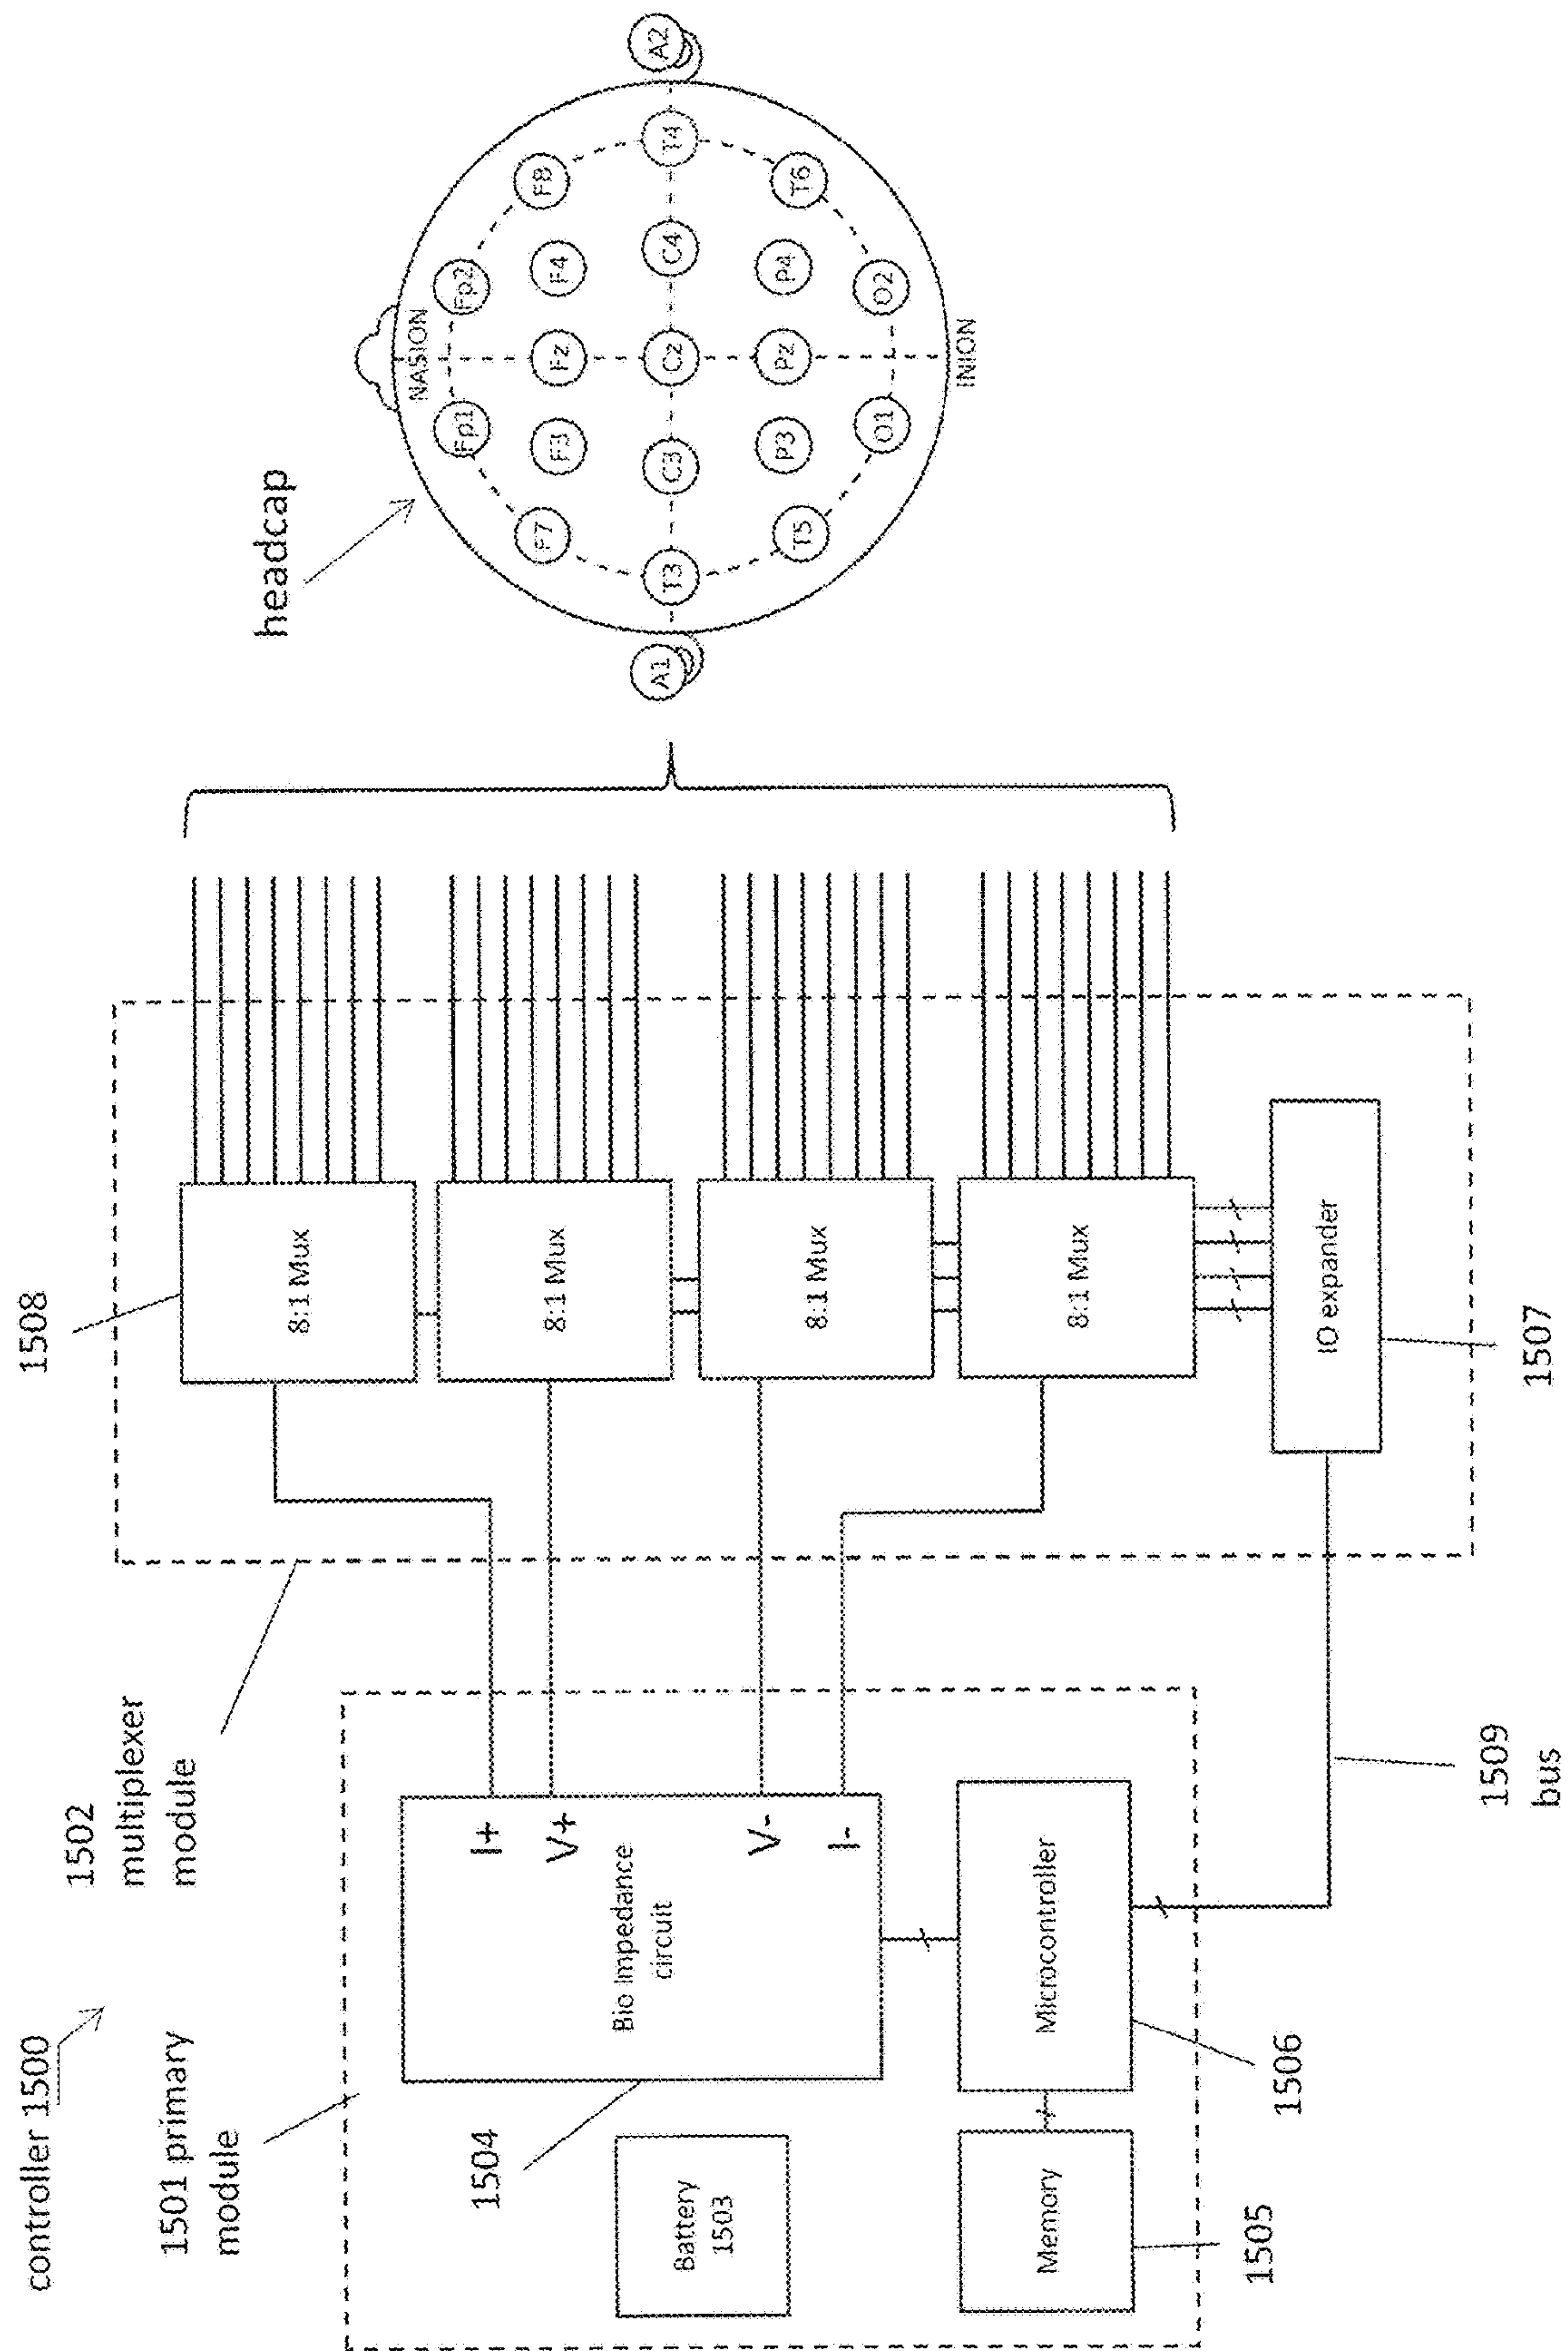


FIG. 14B

Fig 15 - High-Level Architecture and Headset connections



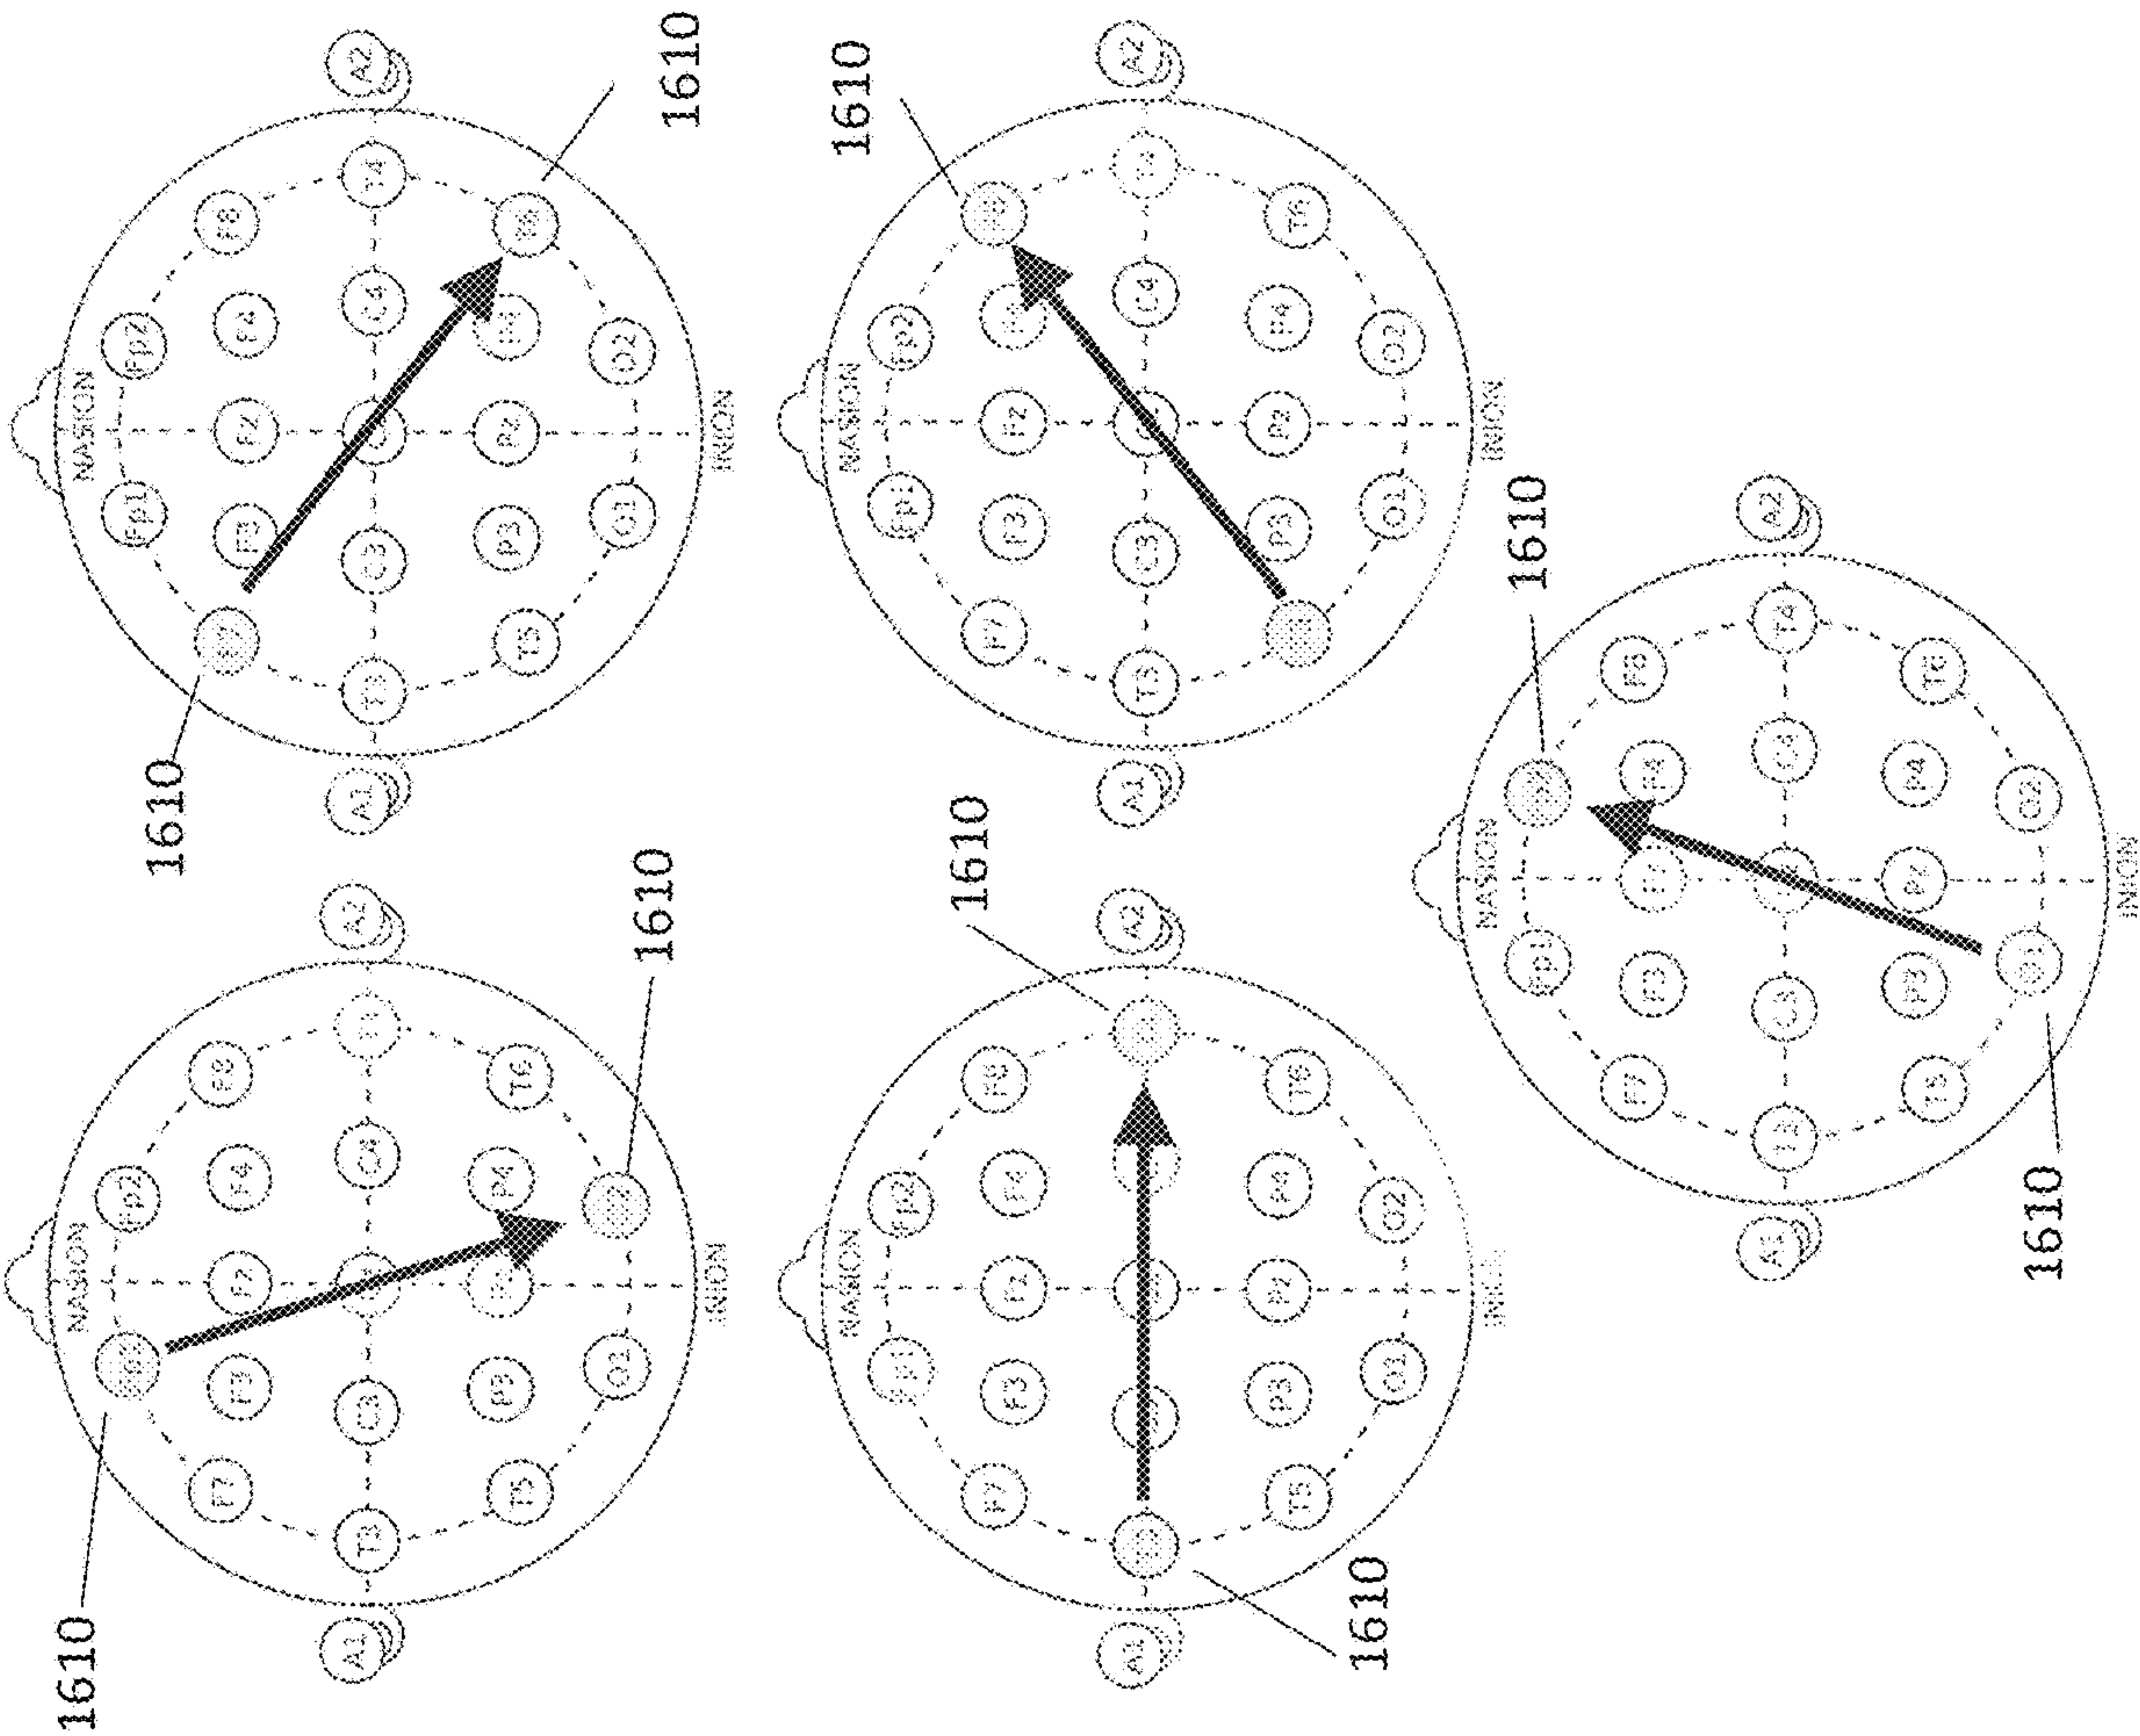


Fig 16 - Current Drive

Fig 17 - Voltage Sense

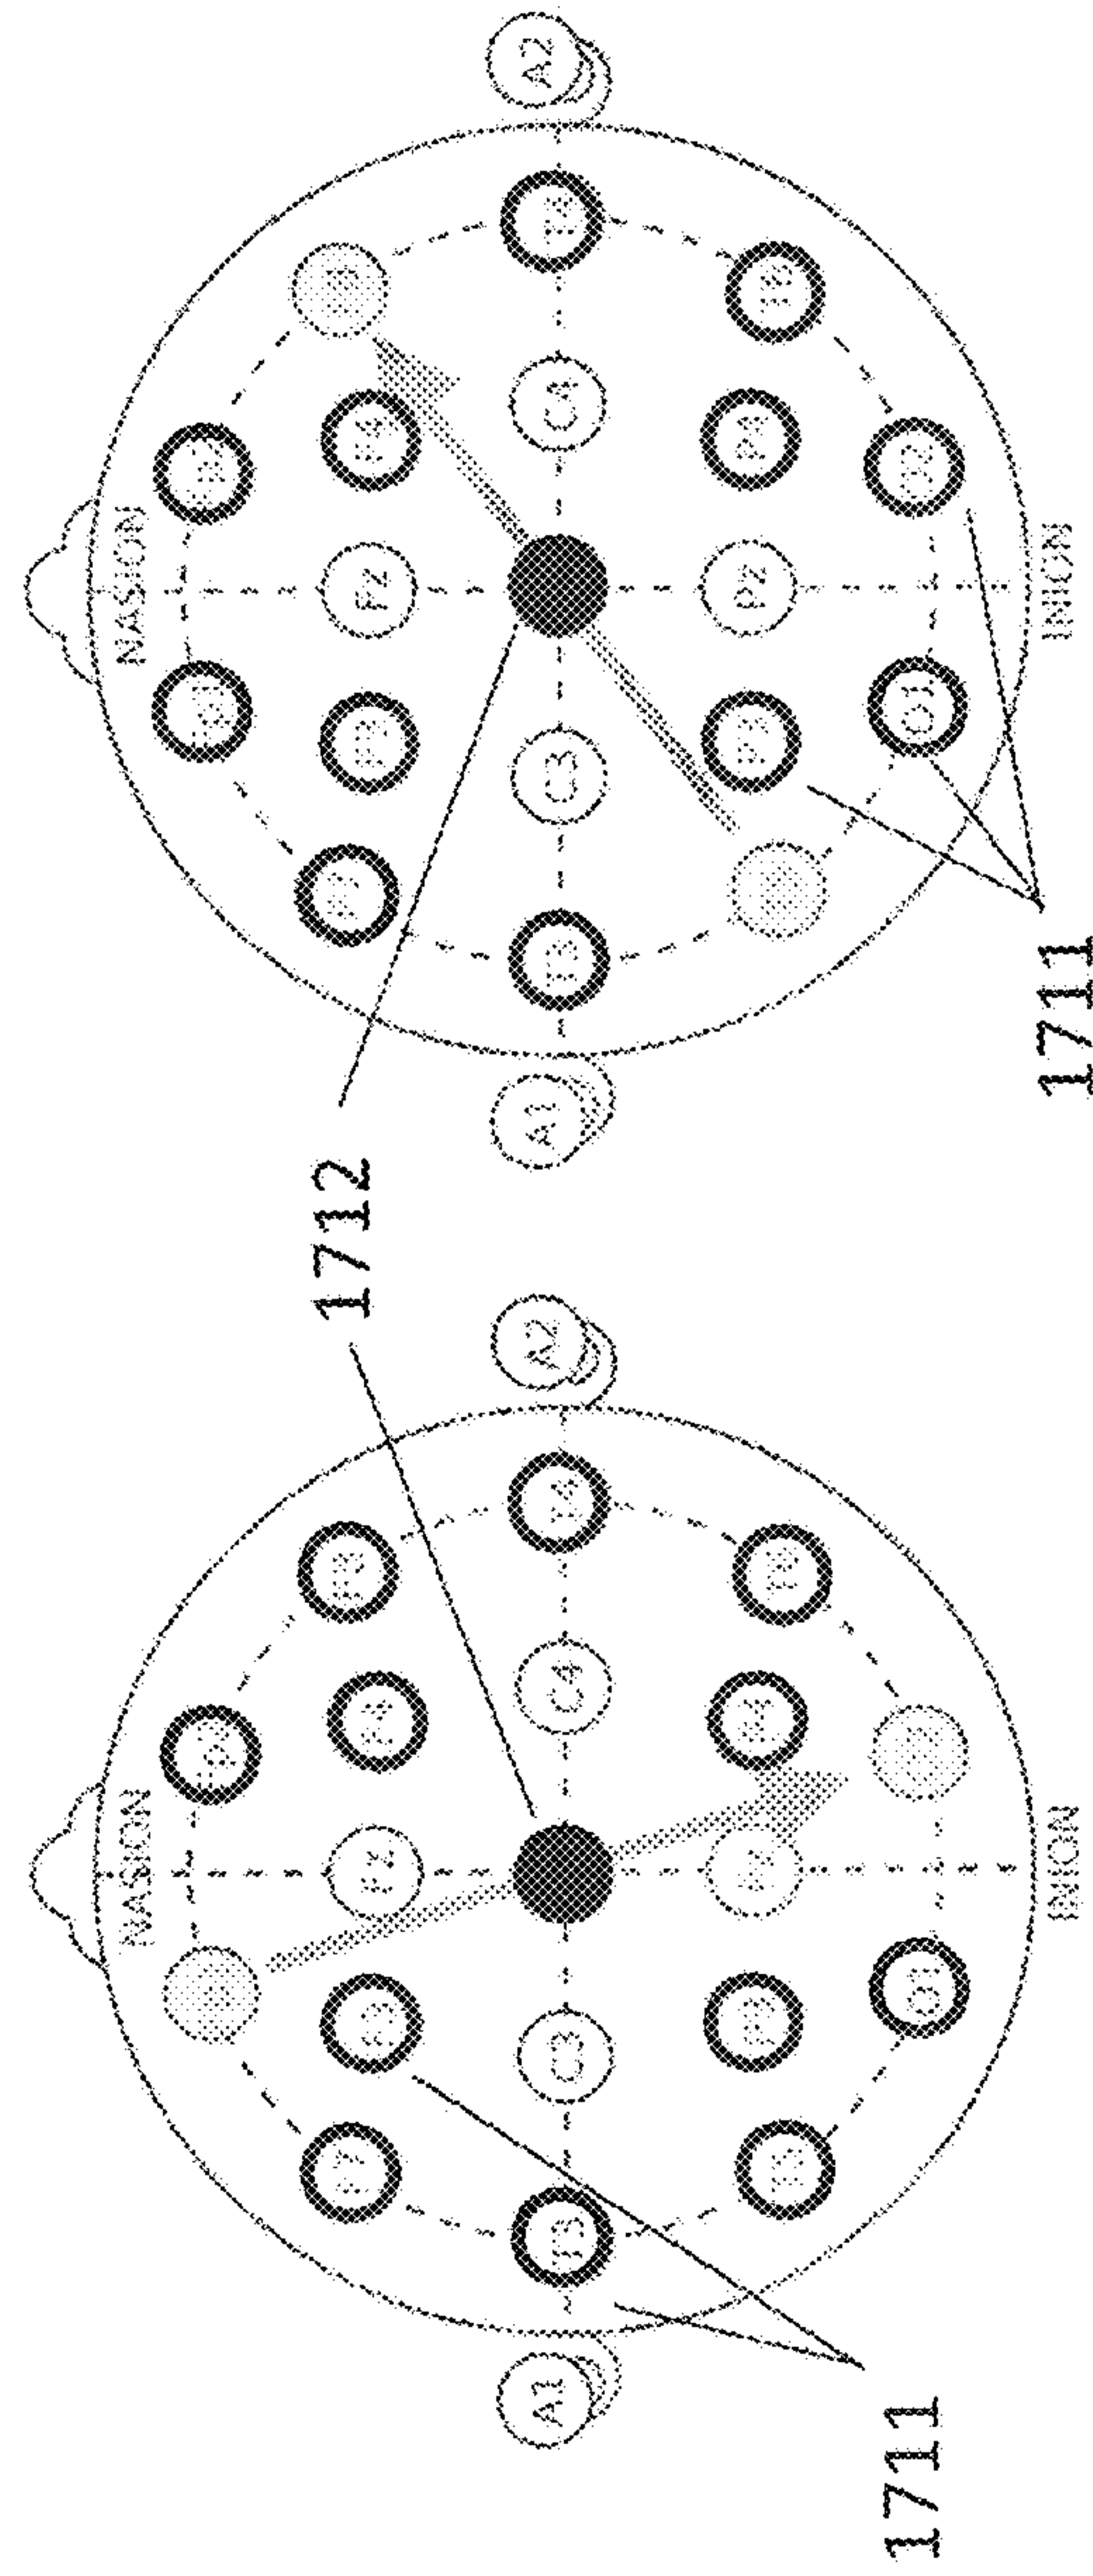


Figure showing potential sense electrodes for two current injection configurations only.

Pin	Electrode	MUX I+	MUX V+	MUX V-	MUX I-
1	Fp1	S1	S1		
2	F7	S2	S2		
3	T3	S3	S3		
4	T5	S4	S4		
5	O1	S5	S5		
6	F3		S6		
7	P3		S7		
8	GND		S8	S8	
9	Fp2			S1	S1
10	F8			S2	S2
11	T4			S3	S3
12	T6			S4	S4
13	O2			S5	S5
14	F4			S6	
15	P4			S7	
16	-				

TMUX1108 MUX	MCP23018 Control Nibble	TMUX1108 MUX Pin	Control bit
V-	GPA0-3	A0	0/4
I-	GPA4-7	A1	1/5
V+	GPB4-7	A2	2/6
I+	GPB0-3	Enable	3/7

FIG 18. Logic Schema


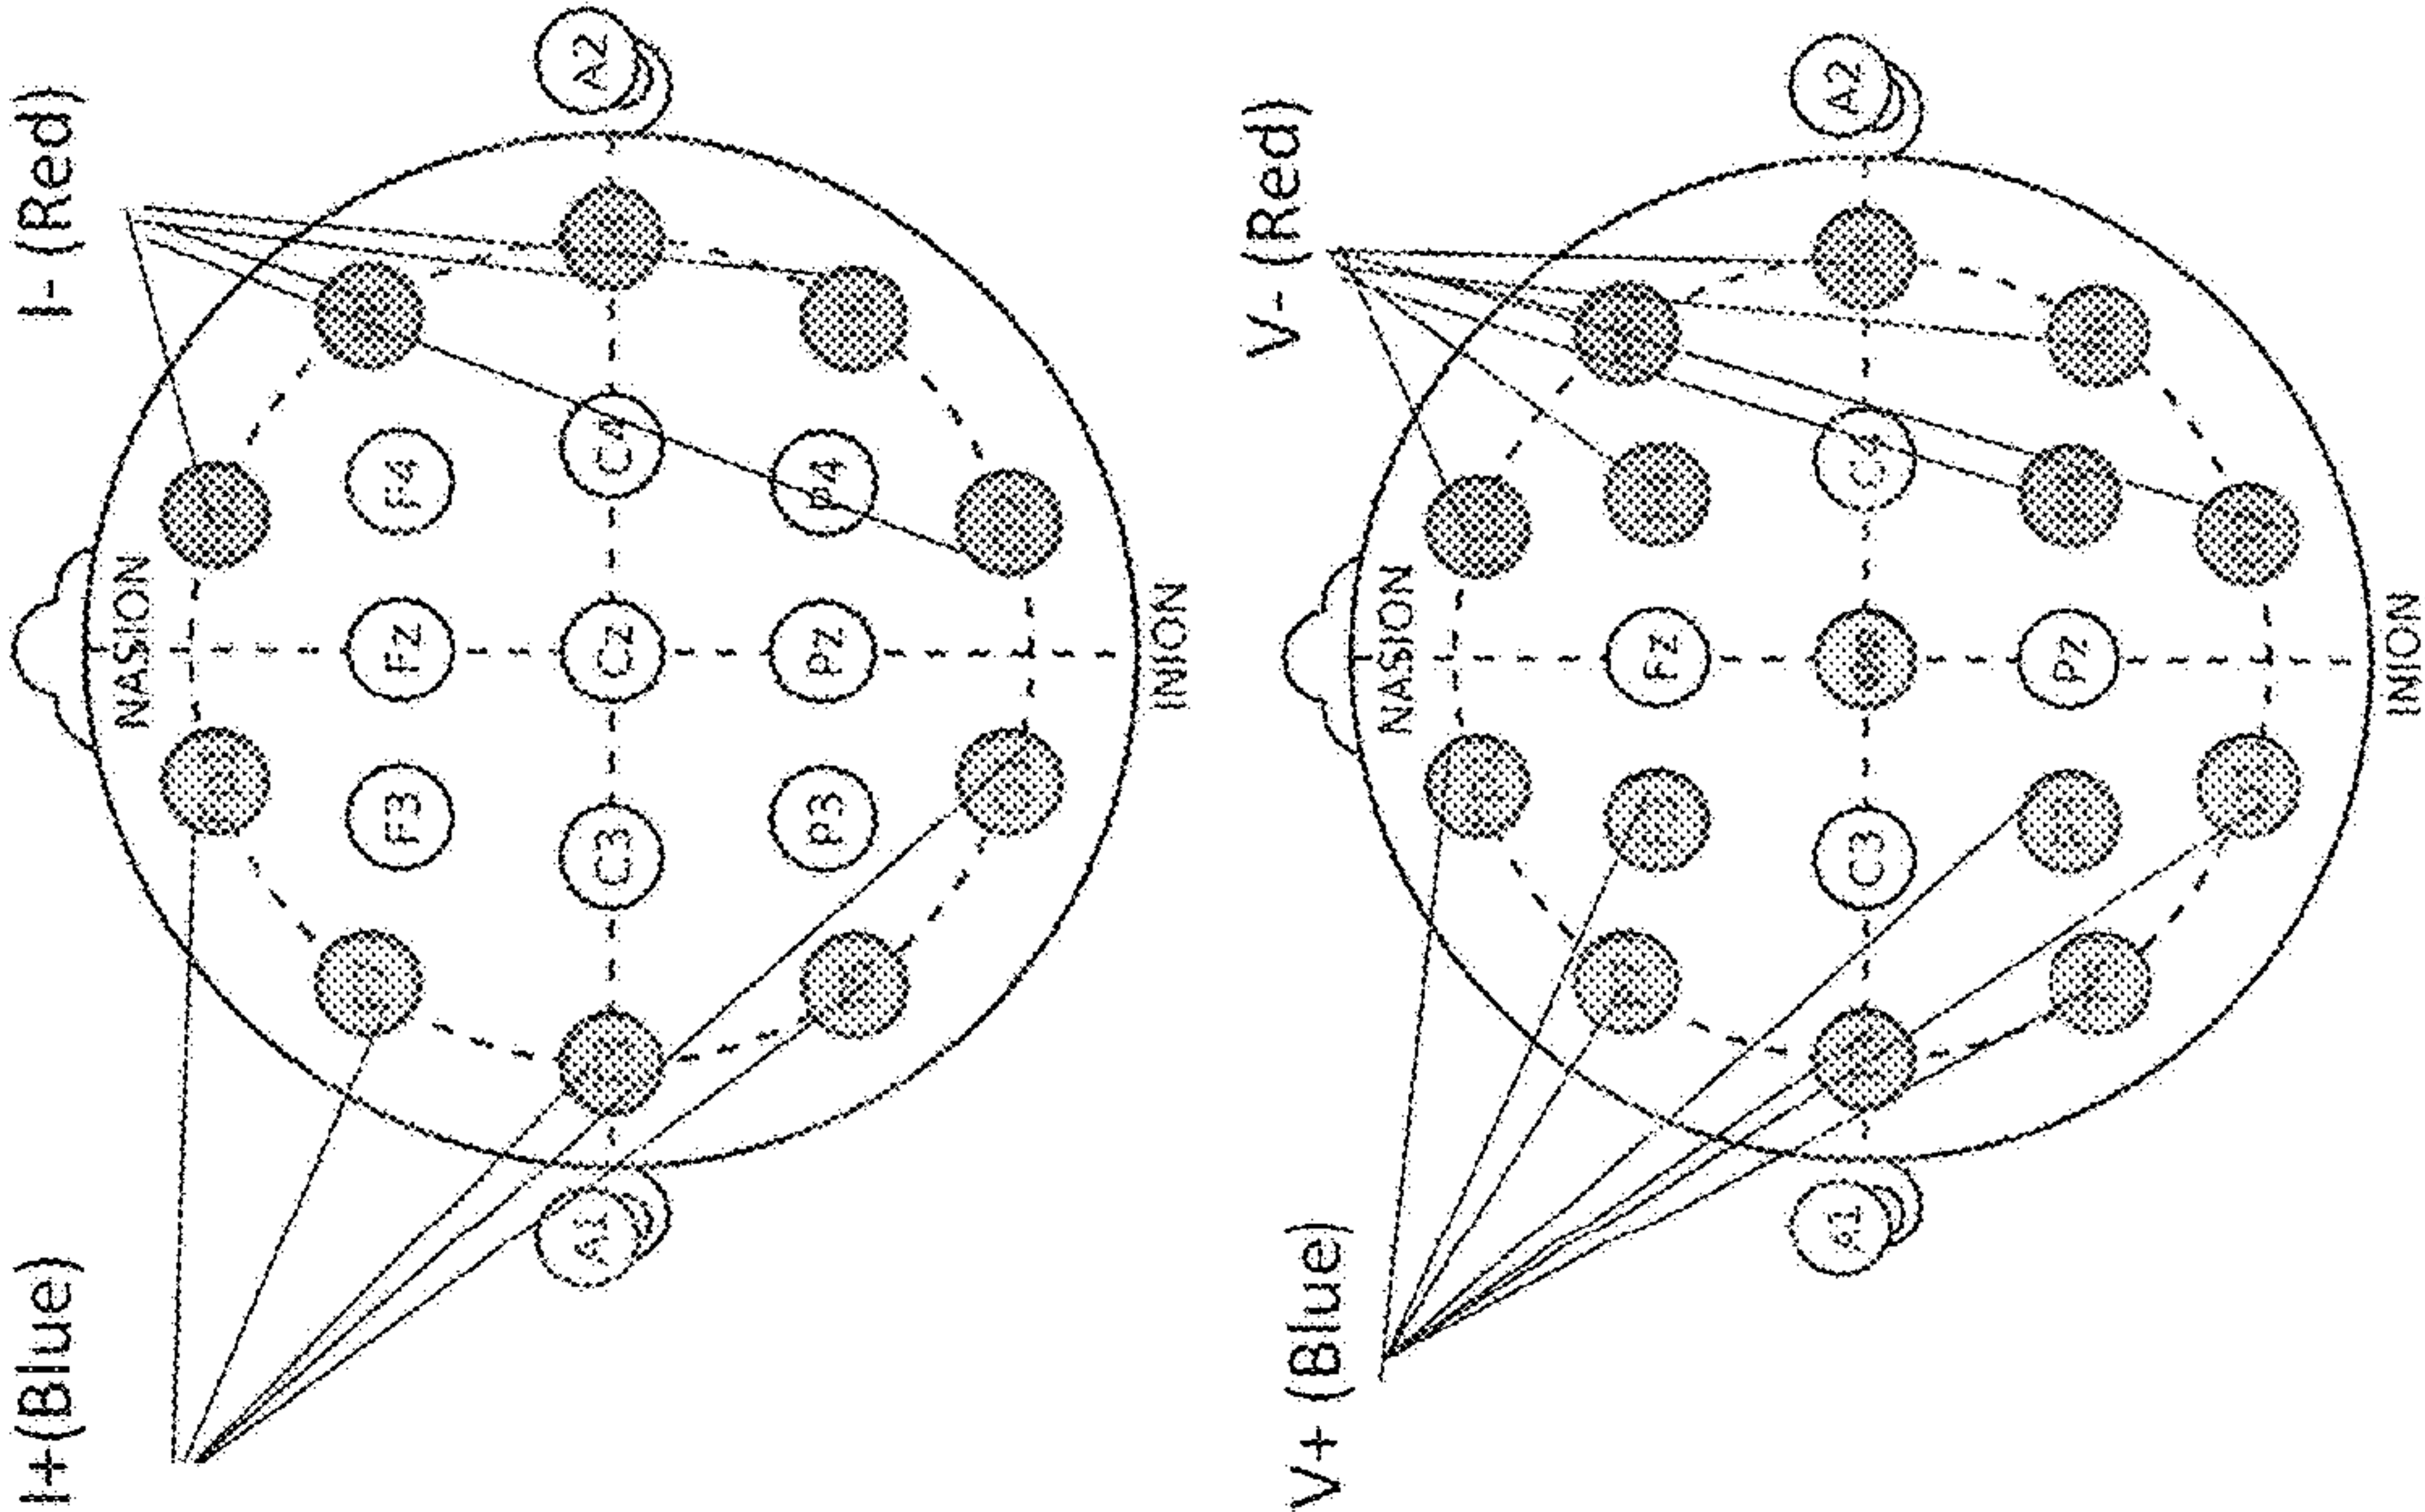


FIG 19. MUX State Machine

Electrodes					Electrodes				
State #	I+	I-	V+	V-	State #	I+	I-	V+	V-
1	Fp1	O2	F7	GND	31	T3	T4	GND	Fp2
2	Fp1	O2	T3	GND	32	T3	T4	GND	F8
3	Fp1	O2	T5	GND	33	T3	T4	GND	T6
4	Fp1	O2	O1	GND	34	T3	T4	GND	O2
5	Fp1	O2	F3	GND	35	T3	T4	GND	F4
6	Fp1	O2	P3	GND	36	T3	T4	GND	P4
7	Fp1	O2	GND	Fp2	37	T5	F8	Fp1	GND
8	Fp1	O2	GND	F8	38	T5	F8	F7	GND
9	Fp1	O2	GND	T4	39	T5	F8	T3	GND
10	Fp1	O2	GND	T6	40	T5	F8	O1	GND
11	Fp1	O2	GND	F4	41	T5	F8	F3	GND
12	Fp1	O2	GND	P4	42	T5	F8	P3	GND
13	F7	T6	Fp1	GND	43	T5	F8	GND	Fp2
14	F7	T6	T3	GND	44	T5	F8	GND	T4
15	F7	T6	T5	GND	45	T5	F8	GND	T6
16	F7	T6	O1	GND	46	T5	F8	GND	O2
17	F7	T6	F3	GND	47	T5	F8	GND	F4
18	F7	T6	P3	GND	48	T5	F8	GND	P4
19	F7	T6	GND	Fp2	49	O1	Fp2	Fp1	GND
20	F7	T6	GND	F8	50	O1	Fp2	F7	GND
21	F7	T6	GND	T4	51	O1	Fp2	T3	GND
22	F7	T6	GND	O2	52	O1	Fp2	T5	GND
23	F7	T6	GND	F4	53	O1	Fp2	F3	GND
24	F7	T6	GND	P4	54	O1	Fp2	P3	GND
25	T3	T4	Fp1	GND	55	O1	Fp2	GND	F8
26	T3	T4	F7	GND	56	O1	Fp2	GND	T4
27	T3	T4	T5	GND	57	O1	Fp2	GND	T6
28	T3	T4	O1	GND	58	O1	Fp2	GND	O2
29	T3	T4	F3	GND	59	O1	Fp2	GND	F4
30	T3	T4	P3	GND	60	O1	Fp2	GND	P4

FIG. 20

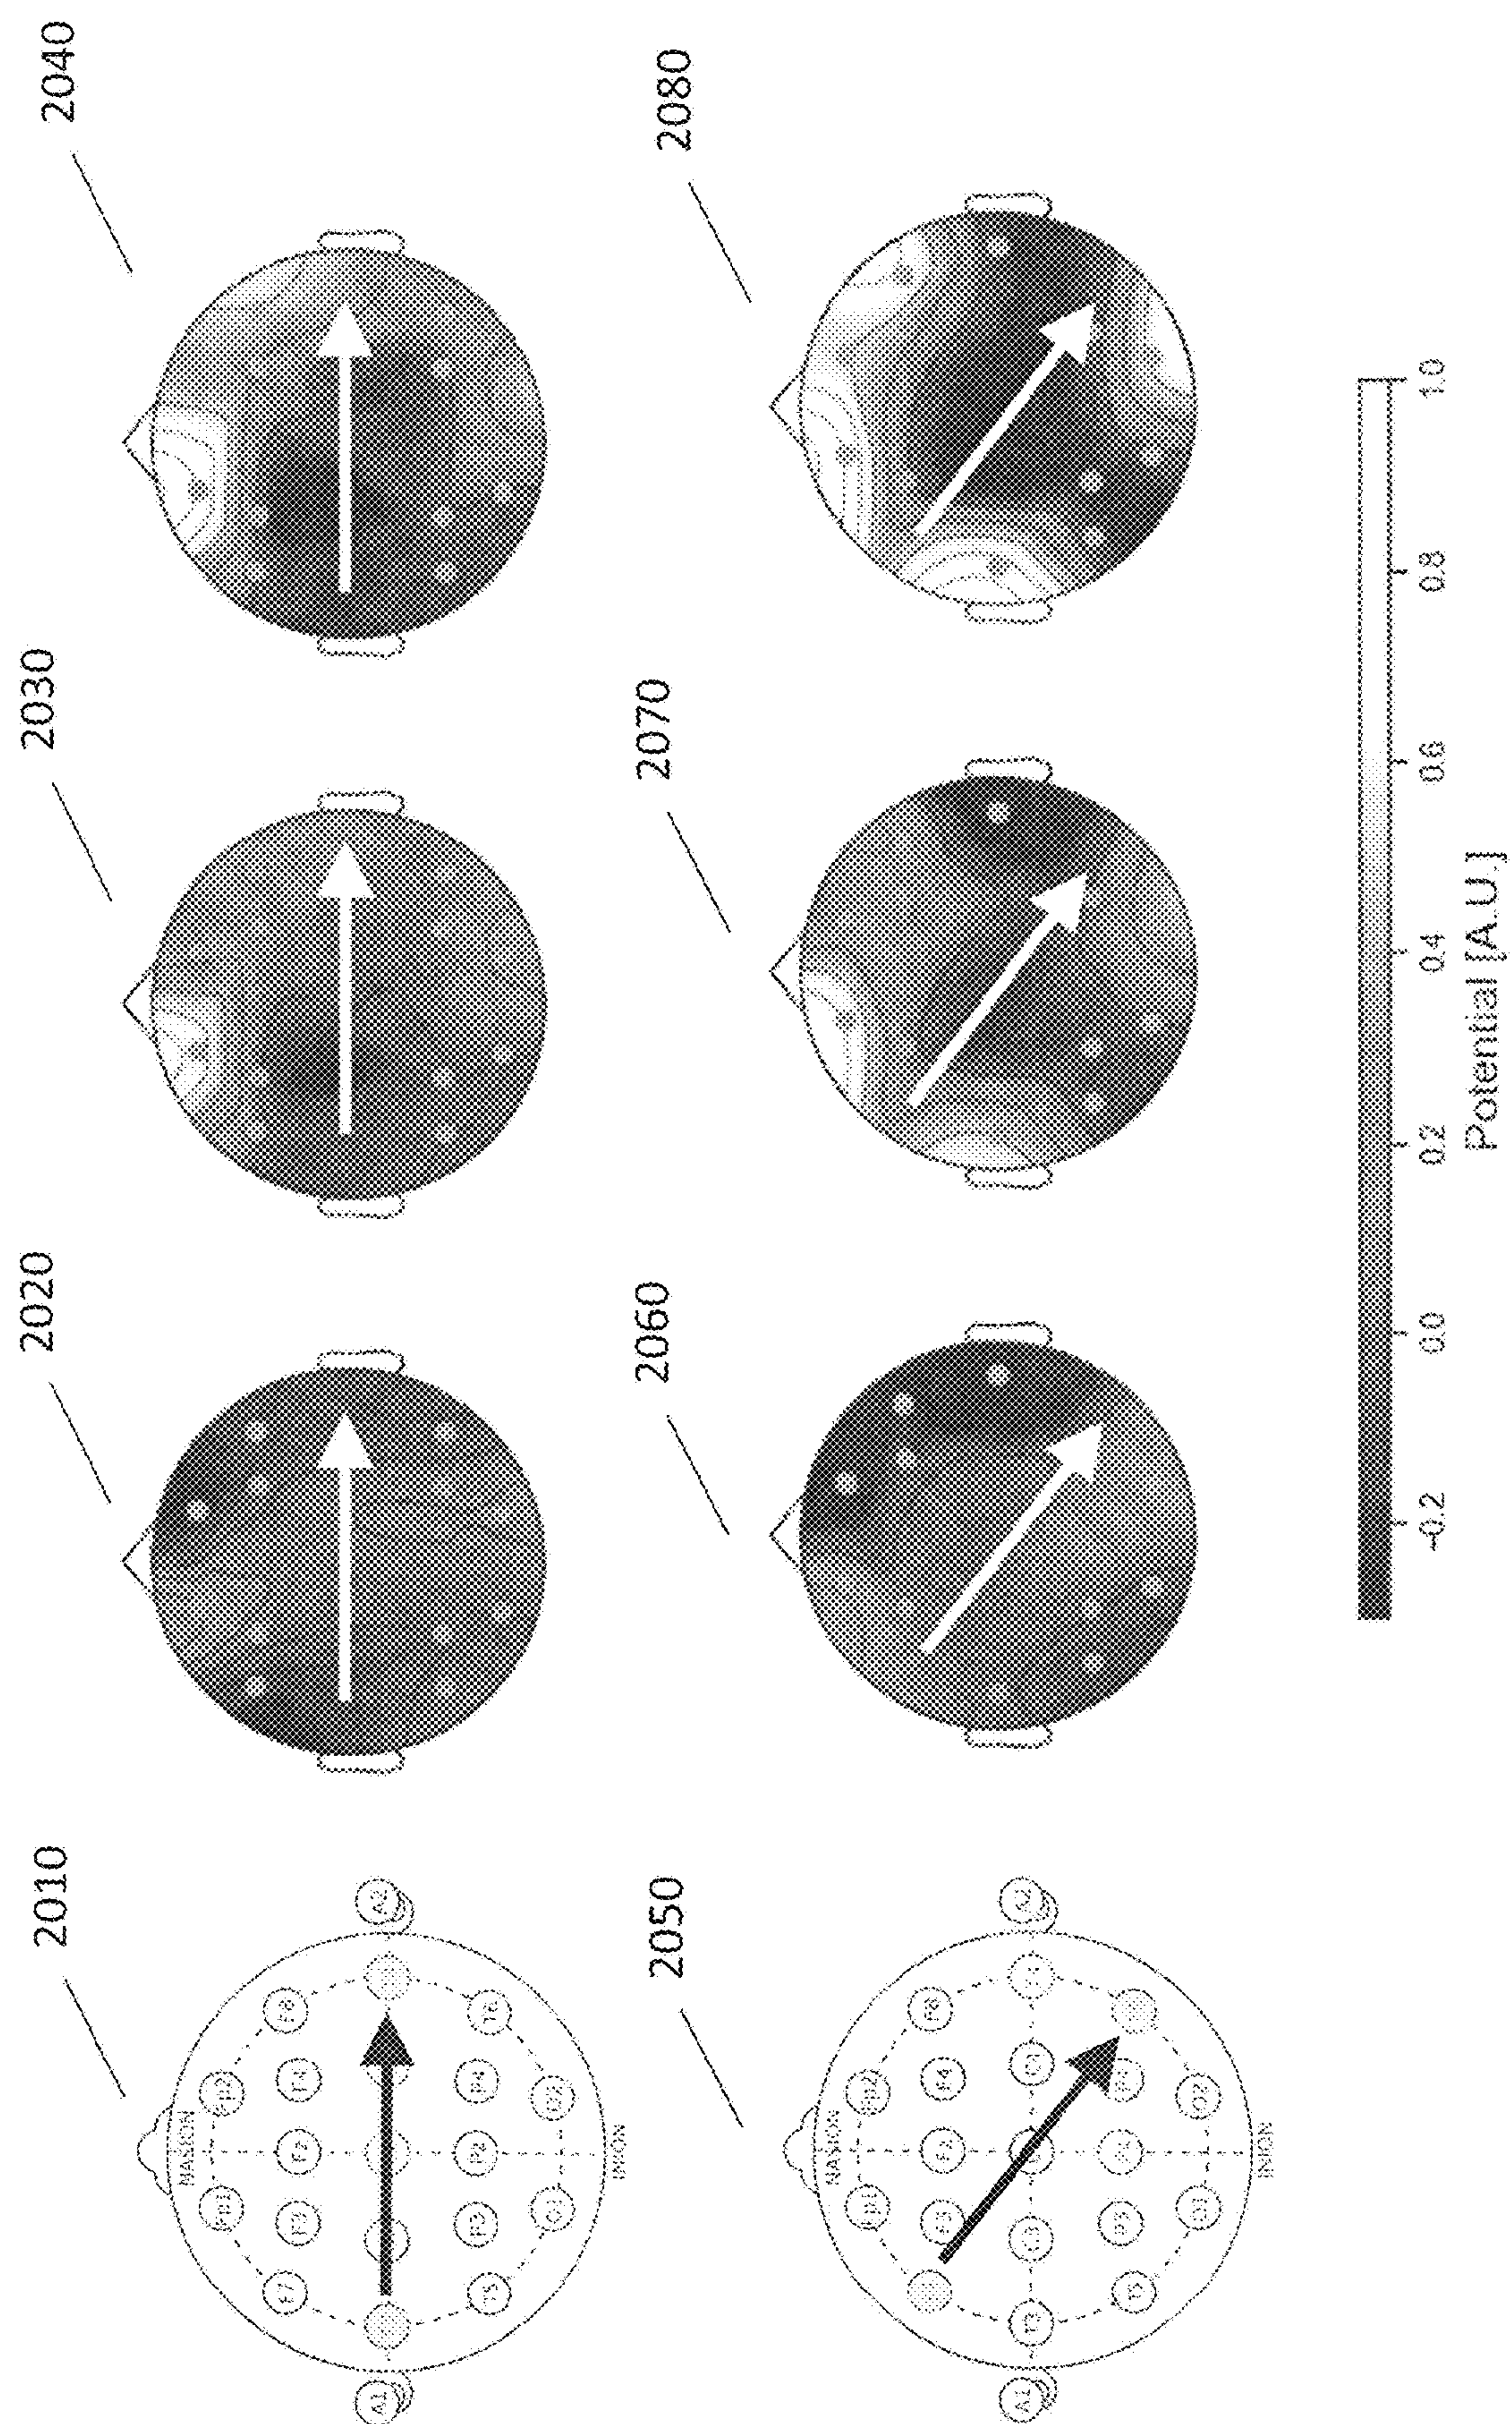

NON-INVASIVE TOPOGRAPHIC LOCALIZATION OF GLYMPHATIC FLOW

CROSS-REFERENCE TO RELATED APPLICATIONS

The present application claims the benefit of U.S. Provisional Patent Application No. 63/380,726 filed Oct. 24, 2022. The present application is related to U.S. patent application Ser. No. 17/937,952 filed Oct. 4, 2022, which is a continuation application of and claims priority to U.S. patent application Ser. No. 17/713,329 filed Apr. 5, 2022, which claims the benefit of U.S. Provisional Patent Application No. 63/244,080 filed Sep. 14, 2021. The entire content of the foregoing applications is incorporated herein by reference.

FIELD OF THE INVENTION

The invention relates generally to the collection of neurophysiology and neurovascular data from a wearable device for use in identifying, predicting, and treating neurodegeneration.

BACKGROUND

Interest in brain fluid transport systems has risen rapidly in recent years with the discovery of the glymphatic system and its role in brain protein clearance involved in neurodegeneration such as amyloid- β . Inhibition of glymphatic flow accelerates protein accumulation and cognitive decline in animal models of Alzheimer's disease, traumatic brain injury and Parkinson's disease. The glymphatic flow is primarily active during sleep and driven by cerebrovascular arterial pulsations, thus, sleep, cerebrovascular integrity and neurovascular coupling are required for clearance of waste products that build up in the awake brain. A reduction in glymphatic flow results in accumulation of protein in the brain that leads to neurodegeneration (known as brain proteinopathy) and which can be detected with neuroimaging or molecular analyses of cerebrospinal fluid or blood plasma. Accordingly, non-invasive techniques for monitoring and analyzing information associated with glymphatic flow and its clearance of protein, with a focus on monitoring the mechanism of glymphatic flow that causes the protein accumulation rather than just reporting the accumulation of protein in the brain as done by neuroimaging or molecular analysis, can be useful in diagnosing and treating neurological degeneration.

SUMMARY

The present disclosure is generally directed to collecting neurophysiology and neurovascular data for use in identifying, predicting, and treating neurodegeneration. In one example embodiment, the disclosure is directed to a method, implemented with one or more computer processors, comprising: (a) accessing, by the one or more computer processors, neurophysiological data and neurovascular data recorded during sleep; (b) executing, by the one or more computer processors, a function mapping from said neurophysiological data and neurovascular data to a target that is a marker of glymphatic flow; and (c) outputting, by the one or more computer processors, a target prediction model based on the function mapping.

In another example embodiment, the disclosure is directed to a system comprising: (a) one or more computer

processors; (b) a neurophysiological data acquisition module configured to measure neurophysiological data; (c) a neurovascular data acquisition module configured to measure neurovascular data; and (d) a transmission module configured to transmit the electroencephalogram data and the neurovascular data to a second computing device.

The foregoing embodiments are non-limiting examples and other aspects and embodiments will be described herein. The foregoing summary is provided to introduce various concepts in a simplified form that are further described below in the detailed description. This summary is not intended to identify required or essential features of the claimed subject matter nor is the summary intended to limit the scope of the claimed subject matter.

BRIEF DESCRIPTION OF THE DRAWINGS

The specific features, aspects and advantages of the present invention will become better understood with regard to the following description and accompanying drawings where:

FIGS. 1A and 1B illustrate an embodiment of the system for non-invasive measurement of brain proteinopathy and neurodegeneration that is comparable to molecular analyses or neuroimaging configured in accordance with the present invention,

FIGS. 2A-2B illustrate an embodiment of the in-ear sensors of the system for non-invasive measurement of brain proteinopathy and neurodegeneration that is comparable to molecular analyses or neuroimaging configured in accordance with the present invention,

FIGS. 2C-2G illustrate the assembly process of the ear device that includes the flex circuit and manufactured soft-silicone components in accordance with the present invention.

FIG. 3 illustrates an example computing environment of the system for non-invasive measurement of glymphatic flow, brain proteinopathy, and neurodegeneration that is comparable to molecular analyses or neuroimaging configured in accordance with the present invention,

FIG. 4 is a functional description of the system in accordance with one embodiment of the present invention,

FIGS. 5A and 5B illustrate example methods associated with the collection of neurophysiology and neurovascular data from a wearable device for use in identifying, predicting, and treating neurodegeneration in accordance with one embodiment of the present invention,

FIGS. 6A-6F illustrate the neurophysiology data acquisition module and example associated data in accordance with one embodiment of the present invention,

FIGS. 7A-7E illustrate the neurovascular data acquisition module and example associated data in accordance with one embodiment of the present invention,

FIGS. 8A-8B illustrate the data acquisition module for a marker of glymphatic flow, a molecular analysis marker or a neuroimaging marker of neurodegeneration and associated images in accordance with an embodiment of the present invention,

FIG. 9 is the learning module of the function mapping from non-invasive neurophysiology and neurovascular input data to target output measurements of glymphatic flow in accordance with one embodiment of the present invention, or is the learning module of the function mapping from input data for a marker of glymphatic flow to target output brain proteinopathy or neurodegeneration measurements from molecular analyses or neuroimaging, in accordance with another embodiment of the present invention,

FIG. 10 is the prediction module of a target marker of glymphatic flow from non-invasive neurophysiology and neurovascular input data in accordance with one embodiment of the present invention, or is the prediction module of a target molecular analysis or neuroimaging of brain proteinopathy and neurodegeneration using input data that are markers of glymphatic flow in accordance with another embodiment of the present invention,

FIGS. 11A-11C illustrate the target engagement module and associated data in accordance with one embodiment of the present invention,

FIGS. 12A, 12B, and 12C illustrate an embodiment of the system for non-invasive measurement of glymphatic flow and neurodegeneration in an over-the-head formfactor that positions the data acquisition sensors used to acquire transcranial impedances over the left and right temporal and parietal brain lobes, configured in accordance with the present disclosure,

FIGS. 12D and 12E illustrate another embodiment of the system for non-invasive measurement of glymphatic flow and neurodegeneration in an over-the-head form factor that positions the data acquisition sensors used to acquire transcranial impedances in front and rear bands over the left and right temporal, parietal, and frontal brain lobes, configured in accordance with the present disclosure,

FIG. 13 illustrates an embodiment of the system for non-invasive measurement of glymphatic flow and neurodegeneration in an over-the-head formfactor that positions the data acquisition sensors used to acquire transcranial impedances in a headcap that extends over the left and right temporal, parietal, and frontal brain lobes, configured in accordance with the present disclosure,

FIGS. 14A and 14B illustrate an embodiment of the system for non-invasive measurement of glymphatic flow and neurodegeneration in an over-the-head formfactor that positions the data acquisition sensors used to acquire transcranial impedances in a plurality of left and right locations around the brain, configured in accordance with the present disclosure,

FIG. 15 illustrates components of a controller for a headcap embodiment of a wearable device in accordance with the present disclosure,

FIGS. 16, 17, 18, and 19 illustrate a method of using the headcap embodiment of a wearable device in accordance with the present disclosure.

FIG. 20 illustrates example data from a headcap embodiment of a wearable device in accordance with the present disclosure in a subject sleeping with the device for 100 minutes.

DETAILED DESCRIPTION OF EXAMPLE EMBODIMENTS

Referencing the glymphatic flow responsible for the clearance of proteins described above, the perivascular spaces (PVS) of the brain are central to the glymphatic fluid transport system. Fluorescent dye-labeled particles that enable visualization of the perivascular spaces reveals that the system comprises periarterial, pericapillary, and perivenular spaces all interconnected into a single network. The glymphatic flow system clears brain interstitial fluid (ISF) waste products such as the proteinopathy proteins through the periarteriolar and perivenular spaces to meningeal lymphatics. The PVS is a site of great importance that is affected by disease processes such as cerebral amyloid angiopathy characterized by perivascular amyloid beta deposits and present in over 90% of Alzheimer's disease

brains. PVS accumulation of p-tau is also observed in Alzheimer's disease and has been demonstrated to be present in arteries, arterioles and veins in the brain. In the glymphatic flow system, cerebrospinal fluid (CSF) enters the periarterial spaces, running in the direction of the blood flow and propelled by arterial wall pulsations. CSF mixes with ISF facilitated by aquaporin-4 (AQP4) water channels that are present at the vascular astrocytic endfeet forming the outer wall of the perivascular spaces. During sleep, arterial pulsations drive CSF bulk flow towards the brain. This process has been shown to be highly dependent on the arousal state and AQP4 expression. With modern neuroimaging techniques, it is now possible to visualize CSF flow and its clearance of proteins in the intact CNS by the second-to-second pulsatile movement of CSF through the ventricular system occurring with each cardiac contraction. Respirations further contribute to this rhythm, adding pulsations at a lower frequency. Superimposed on these acute pulsations is a circadian or diurnal rhythm with maximum CSF production occurring at night during sleep and minimum occurring in the afternoon. MRI studies in animal models using CSF tracers reveal that the glymphatic flow from ISF to subarachnoid CSF is enhanced during NREM sleep.

Sleep has profound effects on most aspects of brain physiology, including glymphatic flow and brain blood volume. In animal models, the amplitude of brain blood volume in non-rapid-eye movement (NREM) sleep doubles compared to the awake state and the amount of total blood volume in the brain changes significantly in the transition from wake to sleep and back to wake, showing that brain blood volume dynamics is coupled to arousal state. These changes in blood volume during sleep are linked to variations in neural activity which drive fluctuations in the diameter of arterioles. The strength of this neurovascular coupling changes with arousal state, increasing substantially during sleep compared to wakefulness and explains the increase in brain blood volume during sleep when neural activity is lower than in the wake state.

The concentration of amyloid- β and tau in the interstitial space and CSF follow a diurnal pattern with both protein concentrations reaching their peak during wakefulness and trough during sleep. A single night of sleep deprivation results in a significant increase in soluble amyloid- β in the brain ISF demonstrated with positron emission tomography (PET) using an amyloid-binding radiotracer. The net concentration of amyloid- β , tau and other proteins in the CSF and ISF reflect the combined effects of diurnal- and state-dependent variations in CSF production rate, ISF volume, ISF turnover rate, and glymphatic flow. Sleep slow-wave delta waves are associated with glymphatic flow and the amplitudes of slow delta waves responsible for effective waste removal during sleep. Sleep deprivation results in stalled glymphatic flow and the accumulation of waste solutes including amyloid- β solutes and other proteins in the brain.

During sleep, glymphatic flow is increased by the action of astrocytes using AQP4 channels that are responsible for the modulation of phases between sleep and awake states. Using membrane channel protein AQP4 and water flux through AQP4, astrocytes can shrink the cell volume of brain parenchyma to increase ISF space by 23% during sleep enabling water and solutes to diffuse into adjacent perivascular spaces. During slow-wave sleep, the increase in ISF space, the opening of gap junction of astrocyte end-feet and

an increase in cerebral hemodynamics creates an environment for exchange of nutrients and elimination of waste between ISF and CSF.

Damage to molecular and cellular components of the glymphatic flow system, to the brain neurovascular integrity and to its neurovascular coupling that occurs with aging, chronic co-morbidities, neurodegenerative diseases and physical brain trauma is closely linked to an increase of tau and amyloid- β in extracellular fluids. The spread of these aggregated proteins in the brain parenchyma leads to worsening clinical symptoms and decline in cognition. Measuring the functional integrity of this system and the pathological accumulation of proteins in the brain ISF requires invasive procedures such as PET scans with radiotracers that bind to the protein of interest or lumbar puncture for CSF extraction and analysis of protein concentrations. The cost and complexity of these procedures limits their use to screen for brain proteinopathies or to monitor their progression. Without access to these tests, practitioners today use clinical assessment and cognitive evaluations to screen, diagnose and monitor neurodegenerative disorders such as Alzheimer's disease. The opportunity to intervene early in the 10-to-20-year pre-clinical period of these disorders is lost as is the ability to evaluate promising new treatments that could slow or stop disease progression. Another challenge with existing invasive test procedures is that they must be done in a hospital or clinic setting by trained technicians. This poses additional patient burden that further reduces the effectiveness of these expensive and time-consuming invasive procedures for monitoring progression of proteinopathy, adjusting care plans and monitoring response to new treatments.

The glymphatic system of protein waste clearance operates during sleep and is dependent on features measurable with sleep electroencephalogram (EEG) and on features that measure neurovascular blood volume, pulsation and coupling. Short term disruption in sleep causes an increase in CSF and ISF waste proteins and long-term disruption leads to formation of ISF protein aggregates with neurodegeneration. A wearable device that can measure the relevant EEG features, brain blood volume changes and arterial pulsations during sleep, transmitting the data to a method and system that can predict CSF and ISF waste protein levels and ISF protein aggregation as can be measured using an existing invasive clinical procedure, would provide a significant advantage to medical screening and monitoring of neurodegenerative proteinopathy and help select appropriate interventions that slow or stop protein accumulation and neurodegeneration. As used herein and as described further below, a "wearable device" is a device worn by a subject comprising one or more sensors for collecting neurophysiological and/or neurovascular data from the subject, a processor, memory, and storage device for storing the collected data, and at least one wireless transmission module enabling the wearable device to transmit the collected data to another computing device. The wireless communication capability of the wearable device allows the wearable device to be self-contained so that it requires no external wiring to other equipment. The wearable device is configured to be worn by the subject while sleeping.

According to the embodiment(s) of the present disclosure, various views are illustrated in FIGS. 1A-11C and like reference numerals are being used consistently throughout to refer to like and corresponding parts of the example embodiments for all of the various views and figures of the drawing. Also, please note that the first digit(s) of the reference numbers in FIG. 1 and FIG. 4 correspond to the Fig. number in which the item or part is described in further detail.

The following detailed description contains many specifics for the purpose of illustration. Any one of ordinary skill in the art will appreciate that many variations and alterations to the following details are within scope of the disclosure. Accordingly, the following example embodiments are set forth without any loss of generality to, and without imposing limitations upon, the claimed invention.

Example embodiments of the present disclosure comprise a system and method that enables non-invasive measurement of brain proteinopathy and neurodegeneration. Such measurements are typically done in a medical facility using sophisticated equipment and involve a molecular analysis of cerebrospinal fluid or neuroimaging, and include proteinopathy proteins amyloid, tau or alpha-synuclein levels in a blood plasma or CSF assay, brain amyloid or tau load on a PET scan, brain atrophy on a structural brain MRI, repeated diurnal assessments to measure net change in proteinopathy protein CSF assay or soluble proteinopathy protein burden from neuroimaging. Example embodiments of the present disclosure teach a novel system and method that acquires sleep neurophysiology data synchronized with neurovascular data. The neurophysiology data includes electroencephalogram (EEG) data. The neurovascular data includes continuous transcranial impedance plethysmography (IPG), carotid pulse transit time (PTT), heart rate variability (HRV) and resting heart rate (RHR). The example embodiments can further perform the step of acquiring one of said molecular analyses or neuroimaging test of neurodegeneration following sleep and learning a function mapping from the sleep neurophysiology and neurovascular data to a molecular analyses or neuroimaging marker of neurodegeneration. Learning the function mapping includes using a loss function to determine relevant features in the sleep data, identifying a set of optimal weights that produce a minimum of the loss function, and creating a function mapping, also referred to as a brain proteinopathy and neurodegeneration prediction model, using the optimal weights. The example embodiments can further include performing the step of applying the learned function mapping to new sleep neurophysiology and neurovascular data to screen for, or monitor, said molecular analyses or neuroimaging marker of neurodegeneration. The example embodiments can further include delivering a therapeutic intervention that targets an aspect of sleep neurophysiology or neurovascular either preceding sleep or during sleep, measuring target engagement or effect on the sleep neurophysiology and neurovascular, and further performing the step of applying the learned function mapping to predict the therapeutic effect on brain proteinopathy and neurodegeneration.

Another embodiment of the present disclosure comprises a system and method that enables a person to monitor the effect of a cardiovascular intervention or activity on a molecular analysis or neuroimaging marker of neurodegeneration, which embodiment teaches a novel system and method for performing the step of recording a cardiovascular intervention or activity data that precedes sleep, further performing the step of recording neurophysiology and neurovascular data during sleep and applying a learned function mapping to predict the therapeutic effect on brain proteinopathy and neurodegeneration of the cardiovascular intervention or activity.

Another embodiment of the present disclosure comprises a system and method that enables a person to monitor the effect of a pharmaceutical or neuromodulation intervention on a molecular analysis or neuroimaging marker of neurodegeneration, which embodiment teaches a novel system

and method for performing the step of recording a pharmaceutical or neuromodulation intervention either preceding sleep or during sleep, further performing the step of recording neurophysiology and neurovascular data during sleep and applying a learned function mapping to predict the therapeutic effect on brain proteinopathy and neurodegeneration of the pharmaceutical or neuromodulation intervention.

Another embodiment of the present disclosure comprises a system and method that enables a person to monitor the effect of a diet intervention on a molecular analysis or neuroimaging marker of neurodegeneration, which embodiment teaches a novel system and method for performing the step of recording a diet intervention that precedes sleep, further performing the step of recording neurophysiology and neurovascular data during sleep and applying a learned function mapping to predict the therapeutic effect on brain proteinopathy and neurodegeneration of the diet intervention.

Another embodiment of the disclosure can be a wearable system comprising a wearable computer with sensors and a wireless communication interface to a mobile computer supporting a wireless network interface which communicates with a second computer including a network interface, each computer further including a processor, a memory unit operable for storing a computer program, an input mechanism operable for inputting data into said computer system, an output mechanism for presenting information to a user, a bus coupling the processor to the memory unit, input mechanism and output mechanism, wherein the wearable system includes various executable program modules stored thereon where when executed are operable to perform functions. The wearable computer with sensors can comprise a neurophysiology data acquisition module with sensors capable of recording EEG, a neurovascular data acquisition module with sensors capable of recording neurovascular data, with the data stored on the wearable computer where when executed records to the memory unit of said wearable computer the neurophysiology and neurovascular sensor acquisition data. A transmission module can comprise a wireless network interface (e.g., a Bluetooth or WiFi radio) as well as instructions stored on said wearable computer where when executed transmit through the wireless network interface the recordings stored in the memory unit to said mobile computer. A second transmission module can also be stored on said wearable computer and comprise a wired network interface as well as instructions where when executed transmit through a bus network interface the recordings stored in the memory unit to a local computer station that further transmits the data to a second computer through a wireless network interface. A learning module can be stored on said second computer where when executed learns a function mapping from said transmitted recording to a molecular analysis or neuroimaging marker of neurodegeneration stored on said second computer, uses a loss function to determine relevant features in said recording, identifies a set of optimal weights that produce a minimum for said loss function, and creates said function mapping using said optimal weights. A brain proteinopathy and neurodegeneration prediction module can also be stored on said second computer where when executed applies the learned function mapping, also referred to as the brain proteinopathy and neurodegeneration prediction model, to a new transmitted recording of sleep neurophysiology and neurovascular sensor data from the wearable computer with sensors, to calculate a predicted value for the molecular analysis or neuroimaging marker of neurodegeneration from

the new transmitted recordings. Thus, the brain proteinopathy and neurodegeneration prediction model can determine a predicted brain proteinopathy and neurodegeneration value from the new recording of data without requiring the invasive imaging or assay procedures described previously.

Another embodiment of the disclosure can be a wearable system comprising a wearable computer with sensors and a wireless communication interface to a mobile computer supporting a wireless network interface which communicates with a second computer including a network interface, each computer further including a processor, a memory unit operable for storing a computer program, an input mechanism operable for inputting data into said computer system, an output mechanism for presenting information to a user, a bus coupling the processor to the memory unit, input mechanism and output mechanism, wherein the wearable system includes various executable program modules stored thereon where when executed are operable to perform functions. In one embodiment, the wearable system can comprise a data acquisition module with sensors capable of recording cardiovascular activity data, with said data stored on the wearable computer where when executed records to the memory unit of said computer the acquisition data. In another embodiment, the wearable system can comprise a data input module capable of recording diet and nutrition data, with said data stored on the mobile computer where when executed records to the memory unit of said computer the data. In another embodiment, the wearable system can comprise a data input module capable of recording drug or neurostimulation data, with said data stored on the mobile computer where when executed records to the memory unit of said computer the data. In any of the preceding embodiments, a transmission module can comprise a communication interface and associated instructions stored on said wearable or mobile computer where when executed transmit through the wireless network interface the recordings stored in the memory unit to said second computer. In any of the preceding embodiments, a module can be stored on said second computer where when executed applies a learned function mapping to said transmitted recording of sleep neurophysiology and neurovascular sensor data from the wearable computer with sensors, to calculate a value for a molecular analysis or neuroimaging marker of neurodegeneration from the transmitted recordings.

The details of the invention and various embodiments can be better understood by referring to the figures of the drawing. FIGS. 1A and 1B illustrate an embodiment of the functional description of the system configured in accordance with the present invention and is not intended to limit scope as one of ordinary skill would understand on review of this application that other configurations could be utilized without departing from the scope of the claimed invention. Referring to FIG. 1, the system can comprise a wearable device that can be attached to a subject's head. In one example, the wearable device can attach to the subject's ear. The wearable device can comprise the previously described neurophysiology and neurovascular data acquisition sensors **200** for non-invasive measurement. As further illustrated in FIG. 1, the wearable device can comprise a data storage, processing and transmission module **300** that stores the sensor data acquired, transforms the data to preliminary measurements of sensor impedance for determining that the sensors are correctly placed and the bladder is correctly pressurized, and can communicate with a mobile computer and/or a local computer, and/or a remote second computer to transmit the data for further processing into measurements of brain proteinopathy and neurodegeneration that are com-

parable to molecular analyses or neuroimaging markers. The non-invasive sensors **200** are connected to module **300** through a form-fitting band **100** that houses electrical conduits, electronically isolating digital from analog sensor signals, an air tube that connects an air bladder in sensor **200** with a piezoelectric pump in **300** and inflates the in-ear portion of the ear device **200** to ensure adequate interfacial contact between the surface sensors and the ear and canal epidermis, and a nitinol band designed to ensure secure fitting of the wearable device. An illustration of the attached device is shown in **110**. It should be understood that in alternate embodiments the components of the wearable device can have other configurations and can attach to the user with other mechanisms. For example, the air bladder can be replaced by another type of bladder that fills with fluid.

FIGS. **2A-2B** illustrate an embodiment of the ear sensors of the system configured in accordance with the present invention and are not intended to limit scope as one of ordinary skill would understand on review of this application that other configurations could be utilized without departing from the scope of the claimed invention. Referring to FIG. **2(a)**, the flex circuit housed by the ear device **200** is illustrated in **210**. Component **212** illustrates positioning of the inertial measurement unit (IMU) that measures milligravitational acceleration capable of perceiving ballistic acceleration in the ear from the blood ejected into the aorta with each cardiac contraction. Component **214** illustrates positioning of the photoplethysmogram (PPG) sensor on the flex circuit so that it is in contact with the ear canal wall. The PPG through measuring the reflection of two wavelengths of infrared light through the ear canal skin is capable of measuring pulsatile changes of ear capillary blood volume with each heart beat and arterial oxygen saturation. Flex circuit leads **216** are terminated on the surface of the ear device **200** to be in contact with two conductive electrodes covering the ear device that can be conductive ink, fabric or other material. Referring to FIG. **2(b)** providing illustration **220**, the 1-layer sections of the flex circuit are designed to flex naturally to accommodate for differences in user ear anatomy, the second layer of the 2-layer sections of the flex is a stiffener applied to the undersurface of the flex circuit to keep the sections stiff so that the active and passive electronic components do not detach with bending, and the 4-layer section has a grounding plane between analog and digital signals to reduce or eliminate electronic coupling resulting in signal corruption.

Referring to FIGS. **2C-2G**, the illustrations **230**, **240**, **250**, **260** and **270** show the assembly process of the ear device that includes the flex circuit **210** and manufactured soft-silicone components illustrated in **230** and **250**. Illustration **240** shows the flex circuit **242** attached to the silicone component **230**. Illustration **250** shows the bladder **252** in the second silicone component that is pressurized, with air or fluid, once inside the ear canal. Through inflation, the PPG sensor **264** is brought into tight contact with the ear canal skin for improved signal-to-noise measurement and further ensures good interfacial contact between the conductive electrodes **272** and **273**, used to measure the neurophysiology electrical currents from the brain and the transcranial bioimpedances, and the ear canal epidermis. Note the ergonomic bend in the second silicone component **252** that mimics the first bend in the human ear-canal. The positioning of the IMU **262** on the device is illustrated in FIG. **2F**.

FIG. **3** illustrates an embodiment of the previously described wearable device illustrated as wearable computing

device **305**, comprising the data storage, processing and transmission module **300** configured in accordance with the present invention and is not intended to limit scope as one of ordinary skill would understand on review of this application that other configurations could be utilized without departing from the scope of the claimed invention. Specifically, the data storage, processing, and transmission module **300** comprises one or more processors **308**, a memory **310**, a storage device **314**, and a transmission module **312**. The components of the data storage, processing, and transmission module **300** are responsible for storing the ear device sensor data, processing the data into preliminary measures of sensor impedance to determine that the sensors are correctly placed and the bladder is correctly pressurized, and transmitting the data for further off-line processing into measurements of brain proteinopathy and neurodegeneration that are comparable to molecular analyses or neuroimaging markers. The example of the wearable computing device **305** in FIG. **3** also illustrates the previously described sensors **200**, such as an IMU and/or PPG, which gather data when positioned in the ears of a patient and which provide the data for storage in the storage device **314**, processing by the processor **308**, and transmission by the transmission module **312**. The input/output device **314** can be a user interface in the form of buttons or a display screen. In other embodiments of the wearable computing device, the input/output device may be omitted.

The example embodiment of FIG. **3** illustrates the wearable computing device **305** capable of wireless communication via wireless links with a mobile computing device **320**, such as a smartphone or tablet, and a local computing device **340**, such as a desktop computer. It should be understood that it is not a requirement to have both a mobile computing device and a local computing device and in alternate embodiments only one of the mobile computing device **320** and local computing device **340** may communicate with the wearable computing device **305**. As illustrated in FIG. **3**, the mobile computing device **320** and the local computing device **340** comprise conventional components that are readily understood, including a processor **322/342**, memory **324/344**, a transmission module **326/346**, an input/output interface **328/348**, and a storage device **330/350**. One or both of the mobile computing device **320** and the local computing device **340** can transmit the data collected by the wearable computing device **305** to a second computing device **360**. The second computing device is typically located remotely and accessed via a wide area network such as the Internet. The second computing device can comprise computing components, such as a processor **362**, memory **364**, transmission module **366**, input/output interface **368**, and storage device **370**. The storage device **370** can store various program modules that are executable by the processor **362**. Specifically, the storage device **370** can comprise a learning software module and a prediction software module. For example, the learning software module can comprise a machine learning algorithm or deep learning algorithm that determines a function mapping from the collected neurophysiological and neurovascular data to a target marker of glymphatic clearance or neurodegeneration. The prediction module can comprise a model based on the function mapping that is used to predict glymphatic clearance or neurodegeneration based on sensor data that is newly collected by the wearable computing device from a patient.

FIG. **4** illustrates an embodiment of the functional description of the system configured in accordance with the present invention and is not intended to limit scope as one

of ordinary skill would understand on review of this application that other configurations could be utilized without departing from the scope of the claimed invention. Referring to FIG. 4, a user's sleep neurophysiology data is captured and recorded by the neurophysiology data acquisition module 600 through sensors positioned on the user's head, such as the previously described sensors positioned in the ear. The neurovascular data acquisition module 700 further captures the user's sleep neurovascular data through sensors positioned on the user's head. As explained previously, the neurophysiology data acquisition module 600 and the neurovascular data acquisition module 700 can be implemented in the wearable device.

In contrast, the brain proteinopathy and neurodegeneration target data acquisition module 800 is an invasive module typically implemented using sophisticated equipment at a medical facility and is responsible for acquiring one or more molecular analysis or neuroimaging markers of neurodegeneration. The marker of interest can be a CSF or plasma assay of one of several brain proteinopathy proteins including amyloid beta 42, tau, alpha-synuclein and neurofilament light that are markers of neurodegenerative disorders, a neuroimaging scan such as PET scan with a radiotracer for the protein of interest, an MRI with contrast agent to measure brain atrophy. The CSF assay or PET scan can be taken after sleep to assay an existing level of CSF protein or protein build up in the brain, or taken both before and after sleep to assay the net change in the protein level that occurred during sleep. The marker can also be an MRI with intrathecal contrast agent injected into the CSF prior to sleep and which is cleared via brain interstitial fluid transport into the meningeal lymphatic and cavernous sinus system during sleep, and the uptake and clearance rate measurable using repeat MRI scanning.

The target marker data measured by module 800 is used by the target learning module 900 to create a target prediction module 1000 that maps new neurophysiology data from module 600 and new neurovascular data from module 700 to a predicted molecular or neuroimaging marker of neurodegeneration for longitudinal monitoring without needing to repeat the invasive measurement of module 800. The target learning module 900 and target prediction module 1000 can be implemented as software that uses a machine learning or deep learning algorithm to provide an output. The target learning module 900 and target prediction module 1000 can be implemented as software executed on one or more remote computers such as the second computer described previously. Target prediction module 1000 can also map sleep neurophysiology data from module 600 and sleep neurovascular data from module 700 taken from a new patient to a molecular or neuroimaging marker of neurodegeneration for non-invasive screening that can be used in medical decision making to evaluate the need for the invasive measurement of module 800. The target engagement module 1100 measures the effect that a putative therapeutic intervention has on the sleep neurophysiology or neurovascular data, or degree of target engagement, and how that effect translates into a change in the predicted molecular or neuroimaging marker of neurodegeneration. The intervention can be one of cardiovascular, diet, sleep, pharmacological or neurostimulation.

FIGS. 5A and 5B illustrate embodiments of the present invention in the form of two methods and are not intended to limit scope as one of ordinary skill would understand on review of this application that other methods could be utilized without departing from the scope of the claimed invention. Referring to FIG. 5A, a method of creating and

applying a target prediction model is illustrated. Beginning with operation 505, a processor of a computing device accesses neurophysiological and neurovascular data recorded while one or more patients were sleeping. The data can be recorded using the previously described wearable device or using other devices. In operation 510, the processor can use a learning software module to determine a function mapping between the recorded data accessed in operation 505 and target marker data. The learning software module can use a machine learning algorithm to determine the function mapping. The target marker data can be data indicating glymphatic flow within the brain. Alternatively, the target marker data can be one of a molecular analysis marker of neurodegeneration or a neuroimaging marker of neurodegeneration such as those described in association with module 800 of FIG. 4. After completing the function mapping, in operation 515 the learning software module outputs a target prediction module. The example method of FIG. 5A can end after operation 515 because the target prediction module can be used in a variety of ways. However, the example method of FIG. 5A continues with operations 520-530 to illustrate one application of the target prediction module. Specifically, in operation 520, neurophysiological and neurovascular data that is newly collected from a patient using the wearable device can be input into the target prediction model to generate a marker of glymphatic clearance or a marker of neurodegeneration. In operation 525, the marker that is output can be used to determine and administer a therapeutic intervention for the patient. In certain embodiments, information pertaining to the therapeutic intervention can be input into the wearable device. Lastly, after the therapeutic intervention has been administered, the wearable device can be used again in operation 530 to collect new data from the patient to determine the efficacy of the therapeutic intervention.

Referring now to FIG. 5B, an example method for operating a wearable device in accordance with the example embodiments of this disclosure is illustrated. Beginning with operation 550, the neurophysiological and neurovascular data sensors of the wearable device can be activated for gathering data while a patient sleeps with the wearable device attached to the patient's ears. For example, the processor of the wearable device can execute a data acquisition module stored in the wearable device's storage module, wherein the data acquisition module controls the operation of the sensors. In operation 555, the sensors of the wearable device, such as the IMU and/or PPG, gather neurophysiological and neurovascular data while the patient sleeps. In operation 560, the wearable device can store the gathered data in the storage device of the wearable device. In some instances, as indicated in operation 565, the wearable device's processor can perform certain initial signal processing on the data gathered by the sensors and store such processed data in the wearable device's storage device. Lastly, in operation 570, the transmission module of the wearable device can manage the transmission of the gathered and/or processed data from the wearable device via a wired or wireless communication link to one or both of a mobile computing device and a local computing device. The mobile computing device and/or local computing device can relay the data from the wearable device to a second computing device that can execute a learning software module and a prediction software module.

FIGS. 6A-6F illustrate an embodiment of the neurophysiology data acquisition module 600 of the system configured in accordance with the present invention and is not intended to limit scope as one of ordinary skill would understand on

review of this application that other configurations could be utilized without departing from the scope of the claimed invention. Referring to FIG. 6A, in **610** raw EEG data is acquired from the user during sleep. The EEG data can be acquired using conventional EEG headcap sensors with a bedside amplifier for recording the signals, or using a wearable device with integrated electronics for amplifying and recording the signal. From the raw EEG signal, various derivations can be analyzed to generate a hypnogram **620** that marks the four stages of sleep, N1, N2, N3 and rapid eye movement (REM) from which additional sleep performance parameters **680** can be derived including total sleep time, sleep onset latency, wake after sleep onset, sleep efficiency and number of awakenings. In **630**, slow wave oscillations in the raw EEG signal are detected and the density (number per minute), amplitude and duration of these oscillations are reported in 30 or 60 second epochs during sleep. In **640**, slow wave activity defined as the relative or absolute power in the EEG signal in the frequency band between 0.5 Hz and 4.5 Hz is computed for every 30 or 60 second epoch and reported. Options for computing the power spectrum include a fast Fourier transform, Welch's periodogram or the multitaper method. In **650**, another sleep EEG element, sleep spindles, are detected in one or more EEG derivations. Sleep spindles occur in two types, fast and slow, depending on the spindle frequency. Spindle density, frequency, duration and amplitude is reported in 30 or 60 second epochs for each type. Both slow wave oscillations or activity, **630** and **640**, and sleep spindles **650** are sleep microstructure markers of glymphatic flow. Finally, in **670** the full power spectral density in the EEG signal is computed in 30 or 60 second epochs and reported.

One or more of the EEG data elements illustrated in FIG. 6A can be used in connection with the target prediction model. For example, the EEG data elements illustrated in FIG. 6A can be used to train the target prediction model. As another example, if the EEG data elements are data that is newly collected after the target prediction model is trained, the EEG data elements can be input into the target prediction model to predict new target markers of neurodegeneration.

Referring to FIG. 6B, **622** is an example sleep hypnogram from an individual during one night EEG recording using a standard 10-20 scalp wet-sensor montage and the results of a C3 to M1 derivative is shown. The sleep hypnogram shows when the individual was awake (W) and in stage N1, N2, N3 or REM sleep in each 30 second epoch. In **642** is illustrated the slow wave activity in the 0.5 to 4.5 Hz bandwidth using a Welch periodogram in 30 second epochs. The slow wave activity is seen to peak during N3 sleep. Important features of the slow wave activity include duration, power and frequency that can be used in connection with the target prediction model. For example, the features of the slow wave sleep elements illustrated in FIG. 6B can be used to train the target prediction model. If the EEG slow wave sleep elements are data that is newly collected after the target prediction model is trained, the EEG slow wave sleep data elements can be input into the target prediction model to predict new target markers of neurodegeneration.

During the same night and for the same individual, simultaneous recordings were made using an ear device comprising modules **100**, **200** and **300** illustrated in FIG. 1A. In FIG. 6C, **624** shows the sleep hypnogram recorded by the ear device and **644** shows the slow wave activity in the 0.5 to 4.5 Hz bandwidth using a Welch periodogram and 30 second epochs.

Referring to FIG. 6D, for the same individual during the same night of EEG recording, sleep microstructure spindle

activity in the 10 to 16 Hz bandwidth using a Welch periodogram in 30 second epochs are illustrated in **652** from the standard 10-20 scalp wet-sensor montage using a C3 to M1 derivative. In **654** is illustrated the same analysis using the sensors from the ear device comprising of modules **100**, **200** and **300** illustrated in FIG. 1A. In both illustrations, peak spindle activity is seen to coincide with stage N2 sleep. Important features of spindle activity include duration, power and frequency. For example, the features of the sleep spindle elements illustrated in FIG. 6D can be used to train the target prediction model. If the EEG sleep spindle elements are data that is newly collected after the target prediction model is trained, the EEG sleep spindle data elements can be input into the target prediction model to predict new target markers of neurodegeneration.

For the same individual during the same night of EEG recording, FIG. 6E illustrates the sensitivity agreement on hypnogram stages and sleep performance parameters between different EEG electrode positions. Illustrated in **682** of FIG. 6F are the sensitivity agreement of hypnogram stages between the C3 to M1 derivative to score the hypnogram and the derivative between the left and right ear electrodes in FIG. 1A illustrated in **200**. Illustrated in **684** of FIG. 6F are the agreement in sleep performance parameters derived from the sleep hypnograms between the C3 to M1 derivative to measure the hypnogram and the derivative between the left and right ear electrodes in FIG. 1A illustrated in **200**. The differences in sensitivity agreement and performance parameters are due to the anatomical differences in the sensor location for measurement highlighting the importance of consistent anatomical sensor placement between uses and across users to extract sleep EEG features for the training the target prediction model and as new inputs to a trained target prediction model to make predict new target markers of neurodegeneration. In-ear lead placement as done by the wearable ear device illustrated in FIG. 1A using anatomically informed ear fittings shown in FIGS. 2C-2G ensure consistent anatomical placement by a user.

FIG. 7A-7E illustrates an embodiment of the neurovascular data acquisition module **700** of the system configured in accordance with the present invention and is not intended to limit scope as one of ordinary skill would understand on review of this application that other configurations could be utilized without departing from the scope of the claimed invention. Referring to FIG. 7A, the same sensors **272** and **273** illustrated in FIG. 2G used for recording in-ear EEG are multiplexed to record at 80 kHz, well above EEG bandwidth, transcranial impedance from left to right ear during sleep. Transcranial impedance tracks fluid changes in the brain that arise during sleep, for example from sleep related changes in glymphatic flow and cerebral spinal fluid production, illustrated in module **710**, and from cardiac pulsations, leading to a beat-to-beat measurable cerebral perfusion pulsation illustrated in module **730**. With each heartbeat, a large fraction of the cardiac output is ejected into the internal carotid and vertebral arteries and delivered to the brain parenchyma. This change in brain blood volume lowers the transcranial impedance and is measurable by the sensors. The amplitude of the impedance waveform and the numerical integration of the impedance waveform pulse are proportional to the volume of blood that is ejected into the brain during that cardiac cycle. The moving average of the transcranial impedance during sleep drifts lower. This drift corresponds to a diurnal fluctuation in brain fluid volume with increased fluid volume during sleep from, for example increases in glymphatic flow and cerebral spinal fluid production, and is measurable by module **710**. A larger drop

between onset of sleep and the sleep nadir of the transcranial impedance correlates with a larger increase in total brain fluid composition that would be expected with greater glymphatic flow. The pulsations recorded by module **730** assist fluid flow through the brain interstitial spaces that promotes glymphatic flow during sleep and protein clearance. The larger magnitude of these pulsations, measured as either their amplitude or numerically integrated area measuring ejection volume, is expected to propel greater glymphatic flow leading to improved clearance. Photoplethysmography sensors located in the ear on the device illustrated in FIG. 1A and illustrated **264** in FIG. 2F, record heart rate variability during sleep in module **750**, resting heart rate by module **770** and sinus arrhythmia that can be used to estimate breathing rate also by module **770**. Heart rate variability during sleep measures the sympathetic-parasympathetic tone of the autonomic nervous system, with lower heart rate variability indicating lower parasympathetic tone and higher sympathetic tone. During sleep, higher sympathetic tone activated by the locus coeruleus in the brain decreases brain interstitial fluid flow and protein biomarker clearance. Higher sleep heart rate variability is expected to lead to greater glymphatic flow and protein clearance. Lower sleep resting heart rate recorded by module **770** is compensated by higher cardiac stroke volume to maintain a tightly regulated cerebral blood flow. A higher cardiac stroke volume results in larger cerebral perfusion pulsations that are measurable by module **730** and increase the propelling forces of glymphatic flow. Conversely, diseases that harden arteries, in particular the arterioles that penetrate the brain parenchyma alongside which run the paravascular spaces containing cerebrospinal fluid that is propelled into the brain parenchyma to drive glymphatic flow, decrease the propelling forces. A decrease in the propelling force is measured by a decrease in the magnitude of the cerebral perfusion pulsation in module **730**. Changes in respiratory rate recorded in module **770** also alters the blood volume pulsations in **730** by affecting venous return to the heart and thereby changing cardiac stroke volume.

One or more of the neurovascular data elements illustrated in FIG. 7A can be used in connection with the target prediction model. For example, the neurovascular data elements illustrated in FIG. 7A can be used to train the target prediction model. As another example, if the neurovascular data elements are data that is newly collected after the target prediction model is trained, the neurovascular data elements can be input into the target prediction model to predict new target markers of neurodegeneration.

Referring to FIG. 7B, **714** shows a sleep recording of the cerebral fluid volume from the transcranial impedance sensors illustrated by **272** and **273** in FIG. 2G for the left in-ear device. The sleep hypnogram illustrated in **712** corresponds to the recorded impedance **714** and shows the decrease in impedance as the patient progresses to deep sleep in stage N2 and N3 (slow wave sleep). The drop in impedance corresponds to an increase in fluid (or water) composition in the brain that corresponds to increase in glymphatic flow through the brain tissue and an accompanying increase in the production of cerebrospinal fluid.

An interval of cerebral perfusion pulsation during sleep for this patient is illustrated in **732** and the corresponding ECG signal in **734**. The cerebral perfusion stroke volume is the difference in impedance between the peak and the trough of a pulsation. A larger difference signifies a greater change in fluid, or water, composition resulting from the heart beat and correlates directly with cerebral stroke volume.

Referring to FIG. 7C, for each 500 second epoch during sleep, the sleep hypnogram is illustrated in **752**, a recording of resting heart rate by module **770** is illustrated in **754** and a recording of resting heart rate variability by module **750** is illustrated in **756**, where in both **754** and **756** are illustrated the recording from the sensors by the wearable device illustrated in FIG. 1A against gold-standard electrocardiogram (ECG) recordings.

Referring to FIG. 7D, the pulse transit time module **790** records a ballistocardiogram (BCG) **791** from the in-ear inertial measurement unit (IMU) illustrated by **262** in FIG. 2F. The BCG I, J and K waveforms are highlighted in the recording **791**. Using a wavelet analysis of the BCG recording, the power of the J waveform is illustrated in **792**, with its peak aligning with the J waveform peak of the BCG. Illustrated in **793** is the PPG waveform recording from the in-ear sensor **264** illustrated in FIG. 2F and **794** illustrates the ECG recording. The IMU, PPG and ECG recordings are time-synchronized by module **790**. A 2.5 second duration close-up of the data illustrated in **791-794** is illustrated in **795** of FIG. 7E. Computation of the pulse-transit time of a cardiac ejection is illustrated in **795**. The maximum blood acceleration is marked by the BCG J-wave **796** and trough of the PPG waveform **797** corresponds to the timing capillary blood engorgement in the ear resulting in a reduction in infrared scatter to the PPG collector. The difference between the timings illustrated in **797** and **796** for that one cardiac cycle is the pulse transit time from the aortic valve to the in-ear sensor. The pulse-wave velocity can be calculated as the vascular distance travelled by the blood from the aortic valve to the in-ear sensor divided by the pulse-transit time. In adults that distance stays fixed and changes in pulse-transit time are inversely related to changes in pulse-wave velocity.

FIGS. 8A and 8B illustrate an embodiment of the glymphatic flow, brain proteinopathy and neurodegeneration target data acquisition module **800** of the system configured in accordance with the present invention and is not intended to limit scope as one of ordinary skill would understand on review of this application that other configurations could be utilized without departing from the scope of the claimed invention. Referring to FIG. 8A, in one embodiment **810**, glymphatic flow imaging can be used with diffusion tensor MRI to measure the glymphatic flow of CSF in the perivascular spaces or can be used with a CSF tracer such as gadolinium that when injected intrathecally is cleared through the brain's extravascular, glymphatic flow, transport. Timing the injection just before the onset of sleep, an MRI scan can be done prior to sleep and once again at the end of sleep. The difference in the intensity of the contrast agent in key regions of interest provides a neuroimaging target of glymphatic system function that occurred during sleep.

In another embodiment **830**, a PET scan can be used with a radiotracer specific for a particular protein of interest and relative standard uptake value (SUVr) that quantifies the proteinopathy build up in the brain. In another embodiment, the radiotracer binds to a soluble form of the proteinopathy protein and the PET scan SUVr quantifies the change in concentration of the soluble protein following sleep.

In another embodiment, MRI **850** can be used to measure changes in brain volume, or degree of neurodegeneration, in anatomical regions of interest such as the hippocampus, entorhinal cortex, thalamus, orbitofrontal, parietal, temporal, anterior, and posterior cingulate and the precuneus

regions over two time points separated by several months to provide an target rate of neurodegeneration for an individual.

In another embodiment **870**, spinal fluid concentration of a proteinopathy protein is assayed either in the morning or both before and after sleep. The absolute concentration levels normed to a population or the diurnal difference in concentration before and after sleep provide a target molecular marker for that protein that measures glymphatic flow as net clearance of the protein and also serves as a marker of brain proteinopathy and neurodegeneration.

In another embodiment **890**, plasma concentration of a proteinopathy protein is assayed either in the morning or both before and after sleep. The absolute concentration levels normed to a population or the diurnal difference in concentration before and after sleep provide a target molecular marker for that protein that measures glymphatic clearance function as net glymphatic clearance of the protein and also serves as a marker of brain proteinopathy and neurodegeneration.

The target marker data acquisition module **800** can be implemented using one of embodiment **810**, **830**, **850**, **870**, or **890**. Alternatively, the target marker data acquisition module **800** can be implemented using a plurality of the embodiments illustrated in FIG. **8** in combination.

Referring to FIG. **8B**, **812** and **814** shows a PET scan and SUVR marker for amyloid protein in two distinct individuals. Illustrated in **816** is the SUVR scale with values near 0 signifying low tracer concentrations that occurs when there is low or no amyloid proteinopathy for the tracer to bind to. Values above 1.5 indicate high tracer concentrations that occur with high amyloid build up. The PET scan illustrated in **812** shows no buildup of amyloid in any of the brain region of interest seen in this coronal slice. In contrast, the scan illustrated in **814** shows significant buildup of amyloid in many regions (indicated by arrows) of interest including orbitofrontal and temporal. Important markers of a PET scan include the SUVR value by region of interest for the protein of interest that can be used in connection with the target prediction model. For example, the markers in the PET scans illustrated in FIG. **8B** can be used as targets in training the target prediction model. Once the target prediction model is trained, new EEG features and neurovascular features can be input into the target prediction model to predict new target markers of neurodegeneration. The target marker data acquisition module **800** can be implemented using one of embodiment **810**, **830**, **850**, **870**, or **890**. Alternatively, the target marker data acquisition module **800** can be implemented using a plurality of the embodiments illustrated in FIG. **8** in combination.

FIG. **9** illustrates an embodiment of the biomarker learning module **900** of the system configured in accordance with the present invention and is not intended to limit scope as one of ordinary skill would understand on review of this application that other configurations could be utilized without departing from the scope of the claimed invention. Referring to FIG. **9**, in one embodiment, **901** input data can be the neurophysiology feature data acquired by module **600**, neurovascular feature data acquired by module **700**, or a combination thereof, and glymphatic flow target data acquired by **810** of module **800**. In another embodiment, **901** input data can be a marker of glymphatic flow acquired by **810** and molecular or neuroimaging target output data acquired by module **800** can be any one of the embodiments described by **830**, **850**, **870** or **890** in FIG. **8A** or a combination thereof. The target marker data can be continuously valued, for example a pseudo-diffusion coefficient to mea-

sure glymphatic flow in mm ²/sec using diffusion tensor MRI, SUVR in a PET scan or picomolar concentrations in spinal fluid molecular assays of protein, or can be categorical valued such as high or low based on thresholding the continuous valued measures using standardized levels for a disease stage. Target neuroimaging marker data can be whole brain values or values for specific regions of interest known to be primarily affected by the specific neurodegenerative disease process. The input training data **901** needs to be carefully collected on a population of 12 or more patients at varying levels of the disease process ranging from unaffected to very affected. Having data representative of patients at different extremes of the disease process gives a range of target marker data values, for example as was shown in in the amyloid PET scan SUVR values in FIG. **8B** for an unaffected patient **812** and a patient with advanced amyloidosis in the brain **814**. These extreme values enable the prediction model and fitting procedure **903** to learn the combination of feature patterns in the neurophysiology data **600** and neurovascular data **700** that correspond to unaffected patients and those that correspond to affected patients. Each patient data needs to be collected concurrently with neurophysiology data and neurovascular data collected together for one or more nights around the time of the target glymphatic flow, molecular or neuroimaging marker data. The device illustrated in FIG. **1** is designed to capture concurrent, time synchronized neurophysiology data and neurovascular data from a patient, and to ensure repeatability of the data acquisition by ensuring consistency of the positioning of all the sensors using the anatomically formed ear device illustrated in FIG. **2G**. Repeating acquisition of the neurophysiology data and neurovascular data over several nights yields additional features for training the prediction model in **903** that improves the bias-variance tradeoff of model fitting and improves predictions. The neurophysiology data and neurovascular data is preprocessed by performing feature extraction as is illustrated in FIGS. **6A-F** and FIGS. **7A-E**.

In **903**, a model and fitting procedure are selected. The model can be one of many known machine learning and deep learning models, including those used in commercially available software packages and services, and the fitting procedure is selected based on the model selected. Random forest, a general-purpose machine learning model, works very well to identify the patterns and ranges of the neurophysiology and neurovascular feature values that best separate, or predict, the target glymphatic flow, molecular or neuroimaging markers. Acquiring the patient training data is expensive and requires an investigational review board approved clinical study. Random forest has the advantage over deep learning models in that it provides good results on a relatively small number of patient data examples. Once the model is learned on a population of patients representative of the target application, predictions of brain glymphatic flow, proteinopathy or neurodegeneration in new, unseen patients can be made from the neurophysiology and neurovascular sleep data acquired by the device illustrated in FIG. **1A** without subjecting a patient to expensive and invasive clinical procedures such as brain MRI, cerebrospinal fluid molecular analysis or PET neuroimaging. This allows the device illustrated in FIG. **1A** to both screen for markers of indicating out-of-range values of glymphatic flow, brain proteinopathy or neurodegeneration and to monitor progression of those markers over time for individuals that screen positive.

Once a model such as random forest is selected, the neurophysiology and neurovascular data are input features

and the target marker data is the target output in the model cross validation **905**. The patient data of **901** is first randomly split into a number of folds, such as five non-overlapping sets. The model in **903** is fit to the data of the first four folds and the fitted model is used to predict the target marker data of the patients in the 5th fold. This procedure is repeated four more times, each time leaving out a new fold of patients and their data, resulting in model predictions of the complete target marker data from the input neurophysiology and neurovascular feature data. In **907** the model is evaluated using a goodness-of-fit metric that can be the root-mean-square between the prediction in **903** and the target marker data. Operations **901-907** can be repeated using several different models to determine which provides the most accurate prediction of the target marker data. The best target prediction model is promoted to **909** where holdout patients and their data, including target marker data that has never been seen by the model, is tested and the prediction model and its performance on the holdout data is outputted in **911**.

FIG. **10** illustrates an embodiment of the target prediction module **1000** of the system configured in accordance with the present invention and is not intended to limit scope as one of ordinary skill would understand on review of this application that other configurations could be utilized without departing from the scope of the claimed invention. Referring to FIG. **10**, in one embodiment, **1001** is new neurophysiology and neurovascular data acquired by modules **600** and **700** from an individual and are inputted into the target prediction model output of **911**. Features are extracted from the data as illustrated in FIG. **6A-F** and FIG. **7A-E**. The new neurophysiology and neurovascular data can be acquired from a new, unseen patient or from a patient that was part of the original training data but the new data is acquired several months or years later to evaluate progression of disease. In operation **1003**, the module executes the target prediction model on the new input data of operation **1001** and outputs a marker of glymphatic flow **1005**. In another embodiment, **1001** is the glymphatic flow output of the target prediction model **1005** and in operation **1003**, the module executes the target prediction model on this new input data of operation **1001** and outputs a marker of brain proteinopathy or neurodegeneration **1005**.

The target prediction can be a predicted value for glymphatic flow, a level of a protein accumulation such as those described previously or a degree of neurodegeneration measured as changes in whole-brain volume or regional volume using structural MRI. The predictions can be continuous values of marker values used to monitor for disease progression or response to intervention, or categorical values to determine the presence or absence of a disease stage. The target predictions of disease stage classification can be submitted for regulatory approval with the appropriate regulatory validation study and reporting of sensitivity, specificity, positive and negative predictive values compared to a gold-standard target such as a molecular analysis or neuroimaging test.

FIG. **11A-C** illustrate an embodiment of the target engagement module **1100** of the system configured in accordance with the present invention and is not intended to limit scope as one of ordinary skill would understand on review of this application that other configurations could be utilized without departing from the scope of the claimed invention. Referring to FIG. **11A**, in one embodiment, the target engagement module **1110** records data from an intervention before sleep or during sleep, module **1130** records the neurophysiology and neurovascular data during sleep and

input data from the intervention in operation **1110**. In module **1150**, engagement of the intervention with one of a neurophysiology target or feature, illustrated in FIG. **6A**, or one of a neurovascular target or feature, illustrated in FIG. **7A**, or a combination of either, is computed as the change in the neurophysiology or neurovascular feature value from baseline. The process **1110**, **1130** and **1150** can be repeated multiple times at different levels or dosing intensities of the therapeutic intervention to establish a target engagement response curve.

The prediction model **911** can be executed using data inputs **1110** and **1130** to output a prediction of the therapeutic intervention's expected impact on glymphatic flow, brain proteinopathy or neurodegeneration in the short term or if sustained in the long term. The glymphatic flow, brain proteinopathy or neurodegeneration prediction that is output can be used to show the effect of the intervention on the glymphatic flow, molecular or neuroimaging marker of neurodegeneration. In other embodiments, operation **1110** can record cardiovascular, diet, pharmaceutical or neuro-modulation interventions, which data is then input into **1130** for execution computation of target engagement at operation **1150**. As such, the effect of the interventions on the neurophysiology and neurovascular data can be ascertained and using the prediction model **911** the intervention's effect on a marker of neurodegeneration determined.

Referring to FIG. **11B**, in one embodiment an input intervention can be raising (reverse Trendelenburg) or lowering (Trendelenburg) the head relative to the feet relative to a flat supine position as illustrated in **1112**. Trendelenburg increases intracranial perfusion pressure. Monitoring the transcranial impedance in **1134** during the interventions of **1112** shows that the transcranial impedance decreased with Trendelenburg and returned to normal as the patient was returned to a flat supine position, demonstrating target engagement of this intervention with cerebral fluid volume. Monitoring the amplitude envelope of in-ear PPG tracing in **1132** shows the reverse occurring with Trendelenburg decreasing the amplitude, or blood volume, going to the ear and scalp and returning to normal when the patient is returned to a flat supine position.

In another embodiment, an input intervention can be a cardiopulmonary intervention such as a Valsalva maneuver or hyperventilation. The transcranial impedance tracing following these two cardiopulmonary interventions are illustrated in **1136** and **1138**. In **1136** the patient performed a 45 second Valsalva maneuver starting at the 1-minute mark. The Valsalva maneuver increases intrathoracic pressure thereby decreasing venous return from the head. The decrease in venous return results in venous engorgement and increase in cerebral fluid volume. This is demonstrated by the decrease in the transcranial impedance during the Valsalva in tracing **1136**. In **1138**, the same patient started hyperventilating lightly at 1 minute and progressed to full hyperventilation at 1 minute and 15 seconds. Each inspiration decreases intrathoracic pressure and increases venous return, causing a decrease in cerebral fluid volume and an increase in transcranial impedance, as shown in tracing **1138**. In both these interventions, monitoring a neurovascular tracing demonstrated target engagement of the intervention with the neurovascular measure, in this case cerebral fluid volume.

Referring to FIG. **11C**, in another embodiment when target engagement of an intervention with one or more of the neurophysiology and neurovascular data has been determined, the prediction model **911** is used to determine the intervention's effect on a marker of glymphatic flow, brain

proteinopathy or neurodegeneration. Illustration **1152** shows rates of clearance of intrathecal gadolinium from the brain measured by serial MRI under three different interventions. The first intervention is control, that is normal sleep with no intervention, the second intervention is sleep deprivation and the third intervention is dexmedetomidine that increases the duration of slow wave sleep. These three interventions engage sleep EEG measures, particularly slow wave sleep duration. Illustration **1152** shows corresponding slower clearance of the contrast agent with sleep deprivation (no slow wave sleep) compared to control, and control shows slower clearance than dexmedetomidine (increased slow wave sleep), as expected from prediction model **911** that is trained on sleep EEG data, neurovascular data and target brain proteinopathy and neurodegeneration data.

Embodiments Set Forth as Clauses

In addition to the forgoing, the various embodiments of the present disclosure include, but are not limited to, the embodiments set forth in the following clauses.

Clause 1. A method implemented with one or more computer processors, the method comprising:

- a. accessing, by the one or more computer processors, neurophysiological data and neurovascular data recorded during sleep;
- b. executing, by the one or more computer processors, a function mapping from said neurophysiological data and neurovascular data to a target that is a marker of glymphatic flow; and
- c. outputting, by the one or more computer processors, a target prediction model based on the function mapping.

Clause 2. The method of clause 1, further comprising:

- a. executing, by the one or more computer processors, a second function mapping from the marker of glymphatic flow to a target that is one of a molecular analysis marker of neurodegeneration or a neuroimaging marker of neurodegeneration; and
- b. outputting, by the one or more computer processors, a target prediction model based on the second function mapping.

Clause 3. The method of clause 1, wherein the neurophysiological data are electroencephalogram recordings, and sleep macrostructure and sleep microstructure features are extracted from the electroencephalogram recordings.

Clause 4. The method of clause 1, wherein the neurovascular data comprise one or more of electrical impedance recordings taken from a patient's head, photoplethysmography measured at the patient's head, and inertial measurement unit acceleration measured in a patient's ear, wherein the neurovascular data are used to compute sleep cerebral fluid volume changes, cerebral perfusion pulsation, heart rate variability, resting heart rate, pulse transit time, pulse wave velocity and respiratory rate.

Clause 5. The method of clause 1, wherein the neurophysiological data and neurovascular data are acquired from a wearable device.

Clause 6. The method of clause 5, wherein sensors of the wearable device are inserted into an ear of a patient and measurements are taken from the ear or ear canal.

Clause 7. The method of clause 6, wherein the wearable device has a bladder that is pressurized inside the ear canal to increase the interfacial surface contact of the sensors to the canal a wall of the ear canal.

Clause 8. The method of clause 2, wherein the molecular analysis marker of neurodegeneration is a CSF or blood plasma assay of one of β -amyloid, tau, p-tau, α -synuclein, and neurofilament light.

Clause 9. The method of clause 2, wherein the neuroimaging marker of neurodegeneration is a PET scan with a radiotracer that binds to one of β -amyloid, tau, or glucose.

Clause 10. The method of clause 2, wherein the neuroimaging marker of neurodegeneration is an MRI scan.

Clause 11. The method of clause 1, further comprising: inputting new neurophysiological data and new neurovascular data into the target prediction model; and outputting a predicted marker of glymphatic flow.

Clause 12. The method of clause 1, further comprising: inputting intervention data into the target prediction model;

inputting new neurophysiological data and new neurovascular data into the target prediction model;

outputting a predicted target marker of glymphatic flow; and

determining an effect of the intervention data on the predicted target marker of glymphatic flow.

Clause 13. A system comprising:

- one or more computer processors;
- a neurophysiological data acquisition module configured to measure neurophysiological data;
- a neurovascular data acquisition module configured to measure neurovascular data; and
- a transmission module configured to transmit the electroencephalogram data and the neurovascular data to a second computing device.

Clause 14. The system of clause 13, wherein the one or more computer processors, the neurophysiological data acquisition module, the neurovascular data acquisition module, and the transmission module are disposed in a wearable device.

Clause 15. The system of clause 14, wherein the wearable device is configured to attach to an ear of a patient.

Clause 16. The system of clause 15, wherein sensors of the wearable device are inserted into the ear and measurements are taken from the ear or ear canal.

Clause 17. The system of clause 16, wherein the wearable device comprises a bladder that is pressurized inside the ear canal to increase interfacial surface contact of the sensors to a wall of the ear canal.

Clause 18. The system of clause 13, wherein the neurophysiological data are electroencephalogram recordings, and sleep macrostructure and sleep microstructure features are extracted from the electroencephalogram recordings.

Clause 19. The system of clause 13, wherein the neurovascular data comprise one or more of electrical impedance recordings taken from a patient's head, photoplethysmography measured at the patient's head, and inertial measurement unit acceleration measured in a patient's ear, wherein the neurovascular data are used to compute sleep cerebral fluid volume changes, cerebral perfusion pulsation, heart rate variability, resting heart rate, pulse transit time, pulse wave velocity and respiratory rate.

Clause 20. The system of clause 13, wherein the second computing device is one of a mobile telephone, a local computing device, and a remote computing device.

Clause 21. The system of clause 13, wherein the second computing device comprises a machine learning algorithm configured to input the neurophysiological data and the neurovascular data and configured to output a target prediction model.

Clause 22. The system of clause 21, wherein the target prediction model is configured to receive as input new neurophysiological data and new neurovascular data and configured to output a predicted marker of neurodegeneration.

Clause 23. The system of clause 21, wherein the target prediction model is configured to receive as input intervention data, new neurophysiological data, and new neurovascular data, and configured to output a predicted marker of brain proteinopathy or neurodegeneration, and a determination of an effect of the intervention data on the predicted marker of brain proteinopathy or neurodegeneration.

Clause 24. A method implemented with one or more computer processors, the method comprising:

- a. accessing, by the one or more computer processors, neurophysiological data and neurovascular data recorded during sleep;
- b. executing, by the one or more computer processors, a function mapping from said neurophysiological data and neurovascular data to a target, the target being one or more of a marker of glymphatic flow, a molecular analysis marker of neurodegeneration, or a neuroimaging marker of neurodegeneration;
- c. outputting, by the one or more computer processors, a target prediction model based on the function mapping;
- d. receiving, as an input, newly collected neurophysiological data and neurovascular data collected during sleep into the target prediction model;
- e. receiving, as an input, data associated with a therapeutic intervention; and
- f. measuring an effect of the therapeutic intervention.

Clause 25. A method implemented with one or more computer processors, the method comprising:

- a. activating a neurophysiological data sensor and a neurovascular data sensor of a wearable device;
- b. gathering, by the sensors, neurophysiological data and a neurovascular data during sleep;
- c. storing the neurophysiological data and the neurovascular data in a storage device of the wearable device;
- d. process the neurophysiological data and the neurovascular data using a processor of the wearable device; and
- e. transmitting, by a transmission module of the wearable device, the neurophysiological data and the neurovascular data to a second computing device.

Clause 26. A non-transitory computer-readable medium comprising computer-executable instructions performing the operations recited in clause 1.

Clause 27. A non-transitory computer-readable medium comprising computer-executable instructions performing the operations recited in clause 24.

Clause 28. A non-transitory computer-readable medium comprising computer-executable instructions performing the operations recited in clause 25.

Additional Examples of Wearable Devices for Measuring Transcranial Impedance

The following description provides additional examples of head-mounted wearable devices that can be used to measure glymphatic flow for the purpose of assessing neurodegeneration. Similar to the examples described previously, the following examples of head-mounted wearable devices use electrodes to measure transcranial impedance. The electrodes can include an input electrode that introduces a small input current at the scalp of the subject wearing the device while sleeping. The wearable device includes additional electrodes that can measure electrical potential at

various locations on the head in response to the input current introduced by the input electrode. The electrical potential measurements are used to identify surfaces of equipotential. The measurements of equipotential are collected over time while the subject sleeps and the time-dependent changes in equipotential provide a measure of glymphatic flow. The frequency of the input current introduced by the input electrode can also be varied to obtain a more complete set of impedance data.

The details of the invention and various embodiments can be better understood by referring to the figures. FIGS. 12A, 12B and 12C illustrate an embodiment of the functional description of the system configured in accordance with the present invention and is not intended to limit scope as one of ordinary skill would understand on review of this application that other configurations could be utilized without departing from the scope of the disclosure. Referring to FIG. 12A, transcranial electrodes for acquiring continuous electrical impedance spectroscopy data can be positioned over different anatomical brain lobes, such as the left frontal lobe 1210 and corresponding right frontal lobe (not visible in FIG. 12A), the left parietal lobe 1220 and corresponding right parietal lobe (not visible in FIG. 12A), and the left temporal lobe 1230 and corresponding right temporal lobe (not visible in FIG. 12A). The system can comprise a wearable device that can be attached to a subject's head and that is designed to position the transcranial electrodes over different transcranial brain lobes. In one example illustrated in FIGS. 12B and 12C, the wearable device 1250 can go over the user's head, similar to headphones, and comprises a left band 1251 and a right band 1256 that are joined at their respective proximal ends by a center band 1255. The distal end of the left band 1251 comprises a left earpiece 1253 that can wrap around at least a portion of the subject's left ear and the distal end of the right band 1256 comprises a right earpiece 1259 that can wrap around at least a portion of the subject's right ear. Although not required, the left earpiece 1253 can include an optional left earbud 1254 that fits within the subject's left ear canal and the right earpiece 1258 can include an optional right earbud 1259 that fits within the subject's right ear canal. When included, the earbuds can be used for proper positioning of the wearable device and can include optional sensors. The center band 1255 can contain a controller for controlling operation of the wearable device. The controller can include a power source (e.g., a battery) for supplying the current to the input electrode. The controller also can include a processor and memory for controlling the power source and processing the electrical potential data measured by the electrodes. The controller can further include a transmission module for wired or wireless communication of data with a nearby computing device such as a mobile phone, tablet, or PC. The inner surfaces of the left band 1251 and the right band 1256 that contact the subject's scalp can include a plurality of impedance spectroscopy electrodes 1275. In some embodiments, the impedance spectroscopy electrodes can also be located along the inner surface of the center band 1255. The power source can supply an input current to one of the electrodes 1275, while other electrodes measure the electrical potential in response to the input current. While gathering impedance measurements during sleep, the controller can vary the electrode providing the input current among the multiple electrodes of the wearable device 1250 in order to gather a broader set of electrical potential measurements. The shape of the wearable device 1250 allows for gathering electrical impedance

25

spectroscopy data across the left and right sides of the head and across the temporal or parietal lobes for non-invasive measurement.

In a second example illustrated in FIGS. 12D and 12E, the wearable device 1260 comprises components similar to the previously described wearable device 1250. Briefly, wearable device 1260 comprises a left front band 1261, a left rear band 1262, a right front band 1266 and a right rear band 1267 that are joined at their proximal ends by a center band 1265. The distal end of the left front band 1261 and left rear band 1262 comprises a left earpiece 1263 that can wrap around at least a portion of the subject's left ear and the distal end of the right front band 1266 and right rear band 1267 comprises a right earpiece 1269 that can wrap around at least a portion of the subject's right ear. Although not required, the left earpiece 1263 can include an optional left earbud 1264 that fits within the subject's left ear canal and the right earpiece 1268 can include an optional right earbud 1269 that fits within the subject's right ear canal. When included, the earbuds can be used for proper positioning of the wearable device and can include optional sensors. The center band 1265 can contain a controller for controlling operation of the wearable device. The controller can include a power source (e.g., a battery) for supplying the current to the input electrode. The controller also can include a processor and memory for controlling the power source and processing the electrical potential data measured by the electrodes. The controller can further include a transmission module for wired or wireless communication of data with a nearby computing device such as a mobile phone, tablet, or PC. The inner surfaces of the left front and rear bands 1261 and 1262 and the inner surfaces of the right front and rear bands 1266 and 1267 can comprise a plurality of electrodes 1276 that contact the subject's scalp and that are used to make the impedance measurements along the subject's head. The controller can select one of the electrodes as the input electrode that provides the input current and other electrodes can measure electrical potential in response to the input current.

Wearable device 1260 differs from wearable device 1250 in that it comprises multiple bands on the left side and multiple bands on the right side that go over the user's head to extend the distribution of the electrodes over the subject's head. In the example illustrated in FIGS. 12D and 12E, two bands are shown on the left side and two bands are shown on the right side. However, other embodiments can include additional bands on each side to further distribute the electrodes over the subject's head. With the impedance spectroscopy electrodes 1276 situated along the inner facing surfaces of the wearable device's left front and rear bands 1261 and 1262 and the right front and rear bands 1266 and 1267, the electrodes contact the subject's head and can acquire impedance spectroscopy data across the temporal, parietal and frontal lobes for non-invasive measurement of glymphatic flow.

FIG. 13 illustrates an embodiment of the electrical impedance spectroscopy sensors of the system configured in accordance with the present invention in a headcap used for clinical electroencephalography (EEG) data acquisition. The illustration is not intended to limit scope as one of ordinary skill would understand on review of this application that other configurations could be utilized without departing from the scope of the disclosure. Referring to FIG. 13, electrodes 1310 are placed over the left frontal lobe, 1320 over the right frontal lobe, 1330 over the left temporal lobe, 1340 over the right temporal lobe, 1350 over the left parietal lobe and 1360 over the right parietal lobe. EEG signals have

26

a unique frequency and are measured passively by the electrodes contacting the subject's head. However, the electrical impedance spectroscopy system multiplexes data acquisition through these electrodes during clinical EEG data acquisition. As explained previously, the electrical impedance measurements are an active, not a passive, technique in that the input current is provided at the input electrode and the responsive electrical potential is measured at other electrodes.

Continuing with the headcap embodiment of the wearable device illustrated in FIG. 13, FIGS. 14A and 14B illustrate an embodiment of techniques for measuring electrical impedance spectroscopy with a headcap used for clinical electroencephalography data acquisition. While not illustrated in FIGS. 13, 14A, and 14B, a controller similar to the controller previously described in FIGS. 12B-12E can be attached to the top or sides of the headcap and electrically coupled to the electrodes. Alternatively, the controller can be separated from the headcap, but electrically coupled to the headcap electrodes by one or more cables that transmit power and data signals between the controller and the electrodes. The illustrations are not intended to limit scope as one of ordinary skill would understand on review of this application that other configurations could be utilized without departing from the scope of the disclosure. Referring to FIG. 14A, the electrical impedance spectroscopy system inputs current over multiple frequencies into left temporal electrode 1410 and with sink right temporal electrode 1420. During current input, the system measures the electrical potential at the remaining electrodes shown in FIG. 14A. This process is repeated across all frequencies selected and throughout the night while the user sleeps to acquire a time-series of impedance spectroscopy data. From the potentials recorded at the sensing electrodes, a finite element model is used to solve for the equipotential surfaces illustrated by 1430 and 1450 overlying the left-brain hemisphere, and 1440 and 1460 overlying the right-brain hemisphere. Other equipotential surfaces can be derived from the electrodes and increasing the number of electrodes over the brain enables higher spatial resolution of the equipotential surfaces. The time-dependence during sleep of these equipotential surfaces is used to measure glymphatic flow and flow shunting across different anatomical areas of the brain.

As illustrated in FIG. 14B, the electrodes for current input and current sink can be rotated to new electrodes 1470 over the left frontal lobe and 1480 over the right posterior temporal lobe. Re-orienting the input and sink electrodes solves for new equipotential surfaces 1490. The input and sink electrodes can be rotated across all pairs of diametrically opposite electrodes, with each new orientation solving for new equipotential surfaces. The time-series changes recorded during a sleep episode in the equipotential surfaces from a specific pair of input-sink electrodes is a measure of brain compartment volume changes and glymphatic flow. Multiplexing electrical impedance spectroscopy with the rotation of input-sink electrodes during a sleep episode, and taking the union of the equipotential surfaces solved in each of the different orientations, gives topographic measures of brain compartment volume changes, glymphatic flow and flow shunting in the brain during sleep.

Referring now to FIGS. 15-19, further details are provided for an example embodiment of a wearable device in the form of a headcap. Similar to the previous example, the electrodes of the headcap described in connection with FIGS. 15-19 can be multiplexed to passively measure EEG signals and to actively measure electrical impedance for assessing glymphatic flow. The illustrations of FIGS. 15-19

are not intended to limit scope as one of ordinary skill would understand on review of this application that other configurations could be utilized without departing from the scope of the disclosure.

FIG. 15 provides further details of a controller 1500 for use with a headcap form of the wearable device of FIGS. 15-19. The controller 1500 also can be used with the previously described wearable devices for measuring transcranial electrical impedance. As explained previously, the controller 1500 can be attached directly to the headcap or can be a separate component that is coupled to the electrodes of the headcap by electrical wires. The controller 1500 comprises a primary module 1501 and a multiplexer module 1502. The primary module 1501 comprises a power source (battery) 1503, a microcontroller 1506, a bioimpedance circuit 1504, and a memory 1505. The battery 1503 supplies power to the components of the controller 1500, including the input current used for the impedance measurements. The microcontroller 1506 executes instructions for controlling the operation of the controller 1500 and the memory 1505 can store executable instructions and impedance data collected from the electrodes. The bioimpedance circuit 1504 is based on a 4-point or Kelvin configuration, with two electrodes/leads inputting a current (I+, I-), and two other electrodes/leads measuring the resulting potential difference (V+, V-). This measurement is performed at one or more frequencies between 100 Hz and 1 GHz. To provide tomographic capabilities, a multiplexer module 1502 expands the connectivity of the bioimpedance circuit 1504 by providing four multiplexers 1508 (8:1, though 16:1 is also possible) that are connected to each of the I+, I-, V+, V- leads to provide dynamic reconfigurability of the drive/sense configuration. These multiplexers are programmed on the fly by the microcontroller 1506. In the case of parallel-programming multiplexers, an Input/Output expander 1507 controlled by an I2C or SPI bus 1509 is used.

The addition of these multiplexers enables changing the current input points (see FIG. 16) while sensing of the scalp potential across most of the scalp surface with respect to a common reference (see FIG. 17). Together with measurement at multiple frequencies, such system provides sequential multifrequency electrical impedance tomography (MFEIT) capabilities.

Referring to FIG. 16, an illustration is provided for collecting impedance measurements using the wearable device of FIG. 15. FIG. 16 illustrates the method of varying the input-sink electrodes. Two multiplexers redirect the input current from the current source leads (I+, I-) to two cap electrodes (1610) chosen from any of the cap electrodes to input the excitation at the subject's scalp current along different vectors, sequentially. The example of controller 1500 using 8:1 multiplexers allows five different vectors to be selected as illustrated in FIG. 16. However, in other embodiments fewer or more pairs of input-sink electrodes can be implemented.

FIG. 17 provides an illustration of the method for measuring electrical potential, from which impedance data can be derived. Two other multiplexers of controller 1500 sequentially connect one of the two sense inputs (V+, V-) of the bioimpedance circuit 1504 to any of the cap electrodes (1711) not used for current input, while the other input is chosen as common reference (1712). The common reference electrode can be a cap electrode or a forehead electrode. Note that a multichannel sensing system can also be used to sense all electrodes simultaneously without the need of multiplexing pairs of sensing electrodes. This would remove

the need for the sensing multiplexers of multiplexer module 1502 coupled to the sense inputs (V+, V-).

The current implementation using 8:1 multiplexers allows 12 electrodes (other than the current input-sink electrodes), spread across the cap to be measured against the reference electrode, providing a homogeneous potential mapping across the head.

Combined with the five current input-sink configurations, this results in a total of 60 different electrical measurements for a given excitation frequency. These 60 different configurations are represented in the MUX State Machine illustrated in FIG. 19 using the logic schema illustrated in FIG. 18. Note that different mux state machines and logic schemas can be used depending on the underlying multichannel analog front end used.

Referring to FIG. 20, example data is shown from a headcap embodiment of a wearable device from a subject sleeping with the device for 100 minutes using the headcap illustrated in FIGS. 14A and 14B, in accordance with the present disclosure. Illustrated in 2010 and 2050 are two orientations of the input current through two pairs of electrodes on the headcap, marked T3 and T4 in 2010 and F7 and T6 in 2050. The input current orientation in 2010 corresponds to MUX State #s 25 through 36 in the MUX State Machine of FIG. 19. The sensing electrodes in these states are Fp1, F7, T5, O1, F3, P3, Fp2, F8, T6, O2, F4, P4 whose locations are shown in 2010. Illustrations 2020, 2030 and 2040 in FIG. 20 show the change in the measured electrical potentials in the sensing nodes from wake to sleep at 10 minutes, 45 minutes, and 90 minutes of sleep, respectively. Input current orientation 2010 reveals a progression of increasing potential in 2020, 2030 and 2040 that corresponds to an increased shift of fluid into the extracellular compartment from 10 minutes to 90 minutes of sleep that begins anteriorly in the left frontal lobe and spreads posterolateral. The input current orientation in 2050 corresponds to MUX State #s 13 through 24 in the MUX State Machine of FIG. 19. Input current orientation 2050 reveals a second progression of increasing potential in 2060 (10 minutes), 2070 (45 minutes), and 2080 (90 minutes) that corresponds to an increased shift of fluid into the extracellular compartment from 10 minutes to 90 minutes of sleep that begins over the left temporal lobe and spreads posteriorly. Shifts in fluid from the brain parenchymal intracellular compartment to the brain parenchymal extracellular compartment during sleep arise because of glymphatic flow. FIG. 20 illustrates that the present embodiment measures both the magnitude of the fluid shift, or glymphatic flow, and the topographic dynamic of the flow by brain region. Increasing the density of the electrodes in the headcap used increases the topographic resolution of the flow during sleep and is consistent with the present embodiment.

Additional Example Embodiments Set Forth as Clauses

In addition to the foregoing, the various embodiments of the present disclosure include, but are not limited to, the embodiments set forth in the following clauses.

Clause 1. A device for topographic localization of glymphatic flow, the device comprising:

- a left band comprising left electrodes along an inner surface of the left band
- a right band comprising right electrodes along an inner surface of the right band;
- a connecting band joining the left band and the right band, the connecting band comprising a controller, wherein

the controller comprises a processor and a power source that are electrically coupled to the left electrodes and the right electrodes for gathering electrical potential data for determining impedance; and

wherein at least one electrode of the left electrodes and the right electrodes is an input electrode that provides input currents over a range of frequencies generated from the power source and wherein other electrodes of the left electrodes and the right electrodes measure electrical potential in response to the input currents.

Clause 2. The device of clause 1, wherein left impedance data and right impedance data derived from the electrical potential data provide an indication of a change in the glymphatic flow that is localized to the left electrodes and the right electrodes.

Clause 3. The device of clause 1, wherein the device generates a topographic image showing a change in glymphatic flow based upon left impedance data and right impedance data derived from the electrical potential data.

Clause 4. The device of clause 1, wherein the controller changes the input electrode from the at least one electrode to a different electrode among the left electrodes and the right electrodes.

Clause 5. The device of clause 4, wherein the device combines the electrical potential data gathered from multiple input electrode configurations into a topographic representation of changes in the glymphatic flow.

Clause 6. The device of clause 4, wherein a processor applies a prediction model to the electrical potential data gathered from multiple input electrode configurations into a topographic representation of changes in the glymphatic flow.

Clause 7. A device for topographic localization of glymphatic flow, the device comprising:

a left front band and a left rear band each comprising left electrodes along an inner surface of the left front band and the left rear band;

a right front band and a right rear band each comprising right electrodes along an inner surface of the right front band and the right rear band;

a connecting band joining the left front band and the left rear band with the right front band and the right rear band, the connecting band comprising a controller, wherein the controller comprises a processor and a power source that are electrically coupled to the left electrodes and the right electrodes for gathering electrical potential data for determining impedance; and wherein at least one electrode of the left electrodes and the right electrodes is an input electrode that provides input currents over a range of frequencies generated from the power source and wherein other electrodes of the left electrodes and the right electrodes measure electrical potential in response to the input currents.

Clause 8. The device of clause 7, wherein left impedance data and right impedance data derived from the electrical potential data provide an indication of a change in the glymphatic flow that is localized to the left electrodes and the right electrodes.

Clause 9. The device of clause 7, wherein the device generates a topographic image showing a change in glymphatic flow based upon left impedance data and right impedance data derived from the electrical potential data.

Clause 10. The device of clause 7, wherein the controller changes the input electrode from the at least one electrode to a different electrode among the left electrodes and the right electrodes.

Clause 11. The device of clause 10, wherein the device combines the electrical potential data gathered from multiple input electrode configurations into a topographic representation of changes in the glymphatic flow.

Clause 12. The device of clause 10, wherein a processor applies a prediction model to the electrical potential data gathered from multiple input electrode configurations into a topographic representation of changes in the glymphatic flow.

Clause 13. A device for topographic localization of glymphatic flow, the device comprising:

a headcap configured to be worn on top of a head of a subject, the headcap comprising left electrodes and right electrodes, wherein the left electrodes and right electrodes are multiplexed to gather EEG signals and transcranial impedance signals; and

a controller coupled to the headcap, the controller comprising a processor and a power source that are electrically coupled to the left electrodes and the right electrodes for gathering electrical potential data for determining impedance; and

wherein at least one electrode of the left electrodes and the right electrodes is an input electrode that provides input currents over a range of frequencies that are generated by the power source and wherein other electrodes of the left electrodes and the right electrodes measure electrical potential in response to the input currents.

Clause 14. The device of clause 13, wherein left impedance data and right impedance data derived from the electrical potential data provide an indication of a change in the glymphatic flow that is localized to the left electrodes and the right electrodes.

Clause 15. The device of clause 13, wherein the device generates a topographic image showing a change in glymphatic flow based upon left impedance data and right impedance data derived from the electrical potential data.

Clause 16. The device of clause 13, wherein the controller changes the input electrode from the at least one electrode to a different electrode among the left electrodes and the right electrodes.

Clause 17. The device of clause 16, wherein the device combines the electrical potential data gathered from multiple input electrode configurations into a topographic representation of changes in the glymphatic flow.

Clause 18. The device of clause 16, wherein a processor applies a prediction model to the electrical potential data gathered from multiple input electrode configurations into a topographic representation of changes in the glymphatic flow.

The invention claimed is:

1. A device for topographic localization of glymphatic flow, the device comprising:

a headcap configured to be worn on top of a head of a subject, the headcap comprising left electrodes and right electrodes, wherein the left electrodes and the right electrodes are multiplexed to gather passive EEG signals and responsive electrical potential data; and

a controller coupled to the headcap, the controller comprising a processor and a power source that are electrically coupled to the left electrodes and the right electrodes;

wherein at least one electrode of the left electrodes and the right electrodes is an input electrode that provides input currents over a range of frequencies that are generated by the power source and wherein other electrodes of the

31

left electrodes and the right electrodes measure the responsive electrical potential data in response to the input currents, and

wherein the device is configured to provide an indication of a change in the glymphatic flow that is localized to the left electrodes and the right electrodes by deriving left impedance data and right impedance data from the responsive electrical potential data over time.

2. The device of claim 1, wherein the device generates a topographic image on an output interface, the topographic image showing a change in glymphatic flow based upon left impedance data and right impedance data derived from the responsive electrical potential data.

3. The device of claim 1, wherein the controller changes the input electrode from the at least one electrode to a different electrode among the left electrodes and the right electrodes thereby generating additional responsive electrical potential data.

4. The device of claim 3, wherein the device combines the responsive electrical potential data and the additional

32

responsive electrical potential data into a topographic representation of changes in the glymphatic flow.

5. The device of claim 3, wherein a processor applies a prediction model to the responsive electrical potential data and the additional responsive electrical potential data gathered from multiple input electrode configurations and generates a topographic representation of changes in the glymphatic flow.

6. The device of claim 1, wherein the left impedance data and the right impedance data derived from the responsive electrical potential data over time is derived by determining equipotential surfaces extending from the left electrodes to the right electrodes.

7. The device of claim 6, wherein the input electrode is coupled with a sink electrode, the sink electrode located on an opposite side of the head of the subject from the input electrode.

* * * * *